

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015007.D
 Acq On : 18 Mar 2020 05:12
 Operator : SY/MD
 Sample : L1940-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	86	rVB	122524	130763	11.80%	1.530%
2	1.579	145	152	165	rBV	97136	116409	10.51%	1.362%
3	2.123	311	321	337	rBV	198759	284410	25.67%	3.328%
4	3.377	710	711	714	rVB	158	42	0.00%	0.000%
5	3.460	734	737	741	rBV2	480	427	0.04%	0.005%
6	3.479	741	743	746	rVB	251	153	0.01%	0.002%
7	3.531	753	759	763	rBV2	549	625	0.06%	0.007%
8	3.553	763	766	769	rVV	251	159	0.01%	0.002%
9	3.586	774	776	778	rBV	201	71	0.01%	0.001%
10	3.750	824	827	833	rBV2	357	352	0.03%	0.004%
11	3.820	847	849	853	rBV2	346	182	0.02%	0.002%
12	3.933	873	884	921	rBV2	41101	172627	15.58%	2.020%
13	4.377	1005	1022	1054	rVB2	182704	447743	40.41%	5.239%
14	4.685	1116	1118	1121	rBV2	289	160	0.01%	0.002%
15	4.733	1129	1133	1134	rBV	282	170	0.02%	0.002%
16	4.907	1186	1187	1188	rBV	161	46	0.00%	0.001%
17	5.074	1221	1239	1265	rBV2	434828	1108008	100.00%	12.964%
18	5.357	1325	1327	1329	rBV	332	147	0.01%	0.002%
19	5.383	1333	1335	1336	rBV	245	124	0.01%	0.001%
20	5.466	1359	1361	1364	rBV	384	195	0.02%	0.002%
21	5.499	1367	1371	1378	rVB2	478	558	0.05%	0.007%
22	5.528	1378	1380	1381	rBV	152	50	0.00%	0.001%
23	5.579	1392	1396	1400	rBV3	609	690	0.06%	0.008%
24	5.643	1402	1416	1438	rBV	360948	707403	63.84%	8.277%
25	6.045	1539	1541	1542	rBV	137	31	0.00%	0.000%
26	6.097	1542	1557	1582	rBV	238124	485964	43.86%	5.686%
27	6.286	1614	1616	1618	rBV	271	171	0.02%	0.002%
28	6.441	1663	1664	1665	rBV	137	39	0.00%	0.000%
29	6.483	1675	1677	1678	rBV	173	52	0.00%	0.001%
30	6.605	1711	1715	1716	rBV	280	197	0.02%	0.002%
31	6.685	1736	1740	1742	rBV	265	153	0.01%	0.002%
32	6.695	1742	1743	1746	rBV	134	52	0.00%	0.001%
33	6.852	1789	1792	1795	rVB	209	118	0.01%	0.001%
34	6.952	1820	1823	1825	rBV2	161	92	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015007.D
 Acq On : 18 Mar 2020 05:12
 Operator : SY/MD
 Sample : L1940-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	7.010	1829	1841	1873	rVV2	119204	214660	19.37%	2.512%
36	7.167	1884	1890	1891	rBV2	645	578	0.05%	0.007%
37	7.338	1929	1943	1973	rBV	555109	960044	86.65%	11.233%
38	7.643	2027	2038	2053	rBV2	82766	142926	12.90%	1.672%
39	7.798	2082	2086	2088	rBV	403	331	0.03%	0.004%
40	7.814	2089	2091	2092	rBV	237	90	0.01%	0.001%
41	7.968	2126	2139	2146	rBV3	799	1935	0.17%	0.023%
42	8.122	2175	2187	2218	rBV2	230226	539609	48.70%	6.314%
43	8.341	2253	2255	2261	rVB4	838	718	0.06%	0.008%
44	8.370	2261	2264	2265	rBV2	426	272	0.02%	0.003%
45	8.437	2282	2285	2287	rBV2	562	301	0.03%	0.004%
46	8.450	2287	2289	2290	rBV2	278	106	0.01%	0.001%
47	8.637	2346	2347	2349	rBV	347	98	0.01%	0.001%
48	8.650	2349	2351	2353	rVB	195	82	0.01%	0.001%
49	8.807	2398	2400	2402	rBV	232	104	0.01%	0.001%
50	8.871	2408	2420	2445	rBV	537503	887243	80.08%	10.381%
51	9.064	2477	2480	2483	rBV2	428	312	0.03%	0.004%
52	9.087	2485	2487	2489	rVB	400	148	0.01%	0.002%
53	9.296	2548	2552	2554	rBV2	302	230	0.02%	0.003%
54	9.408	2583	2587	2589	rBV	285	261	0.02%	0.003%
55	9.489	2606	2612	2616	rBV	302	372	0.03%	0.004%
56	9.566	2634	2636	2637	rBV2	334	135	0.01%	0.002%
57	9.823	2715	2716	2717	rBV	200	47	0.00%	0.001%
58	9.971	2760	2762	2763	rBV	151	39	0.00%	0.000%
59	10.032	2779	2781	2784	rBV2	387	234	0.02%	0.003%
60	10.068	2790	2792	2794	rVB	362	171	0.02%	0.002%
61	10.238	2833	2845	2861	rBV	364911	574191	51.82%	6.718%
62	10.402	2894	2896	2901	rVB2	640	299	0.03%	0.003%
63	10.936	3061	3062	3065	rVB2	493	194	0.02%	0.002%
64	10.952	3065	3067	3070	rBV2	170	111	0.01%	0.001%
65	11.203	3140	3145	3154	rVB4	1183	1489	0.13%	0.017%
66	11.270	3154	3166	3183	rBV	539842	844984	76.26%	9.887%
67	11.460	3223	3225	3226	rBV	273	101	0.01%	0.001%
68	11.508	3237	3240	3241	rBV	431	233	0.02%	0.003%
69	11.646	3270	3283	3304	rBV	576558	904252	81.61%	10.580%
70	11.897	3360	3361	3363	rBV	244	87	0.01%	0.001%
71	12.019	3397	3399	3400	rBV	221	83	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015007.D
 Acq On : 18 Mar 2020 05:12
 Operator : SY/MD
 Sample : L1940-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	12.090	3419	3421	3424	rVB	410	166	0.01%	0.002%
73	12.373	3506	3509	3513	rBV	253	157	0.01%	0.002%
74	12.415	3520	3522	3526	rBV	252	139	0.01%	0.002%
75	12.473	3537	3540	3541	rBV	267	123	0.01%	0.001%
76	12.691	3604	3608	3610	rBV	358	283	0.03%	0.003%
77	12.984	3696	3699	3701	rBV	338	209	0.02%	0.002%
78	13.190	3760	3763	3767	rBV2	391	306	0.03%	0.004%
79	13.286	3785	3793	3805	rBV4	5793	8144	0.74%	0.095%
80	13.373	3817	3820	3823	rBV2	427	279	0.03%	0.003%
81	13.621	3893	3897	3899	rBV2	556	367	0.03%	0.004%
82	13.875	3975	3976	3980	rBV2	557	302	0.03%	0.004%
83	14.633	4209	4212	4215	rBV	935	683	0.06%	0.008%


Sum of corrected areas: 8546611

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015007.D
Acq On : 18 Mar 2020 05:12
Operator : SY/MD
Sample : L1940-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D89

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

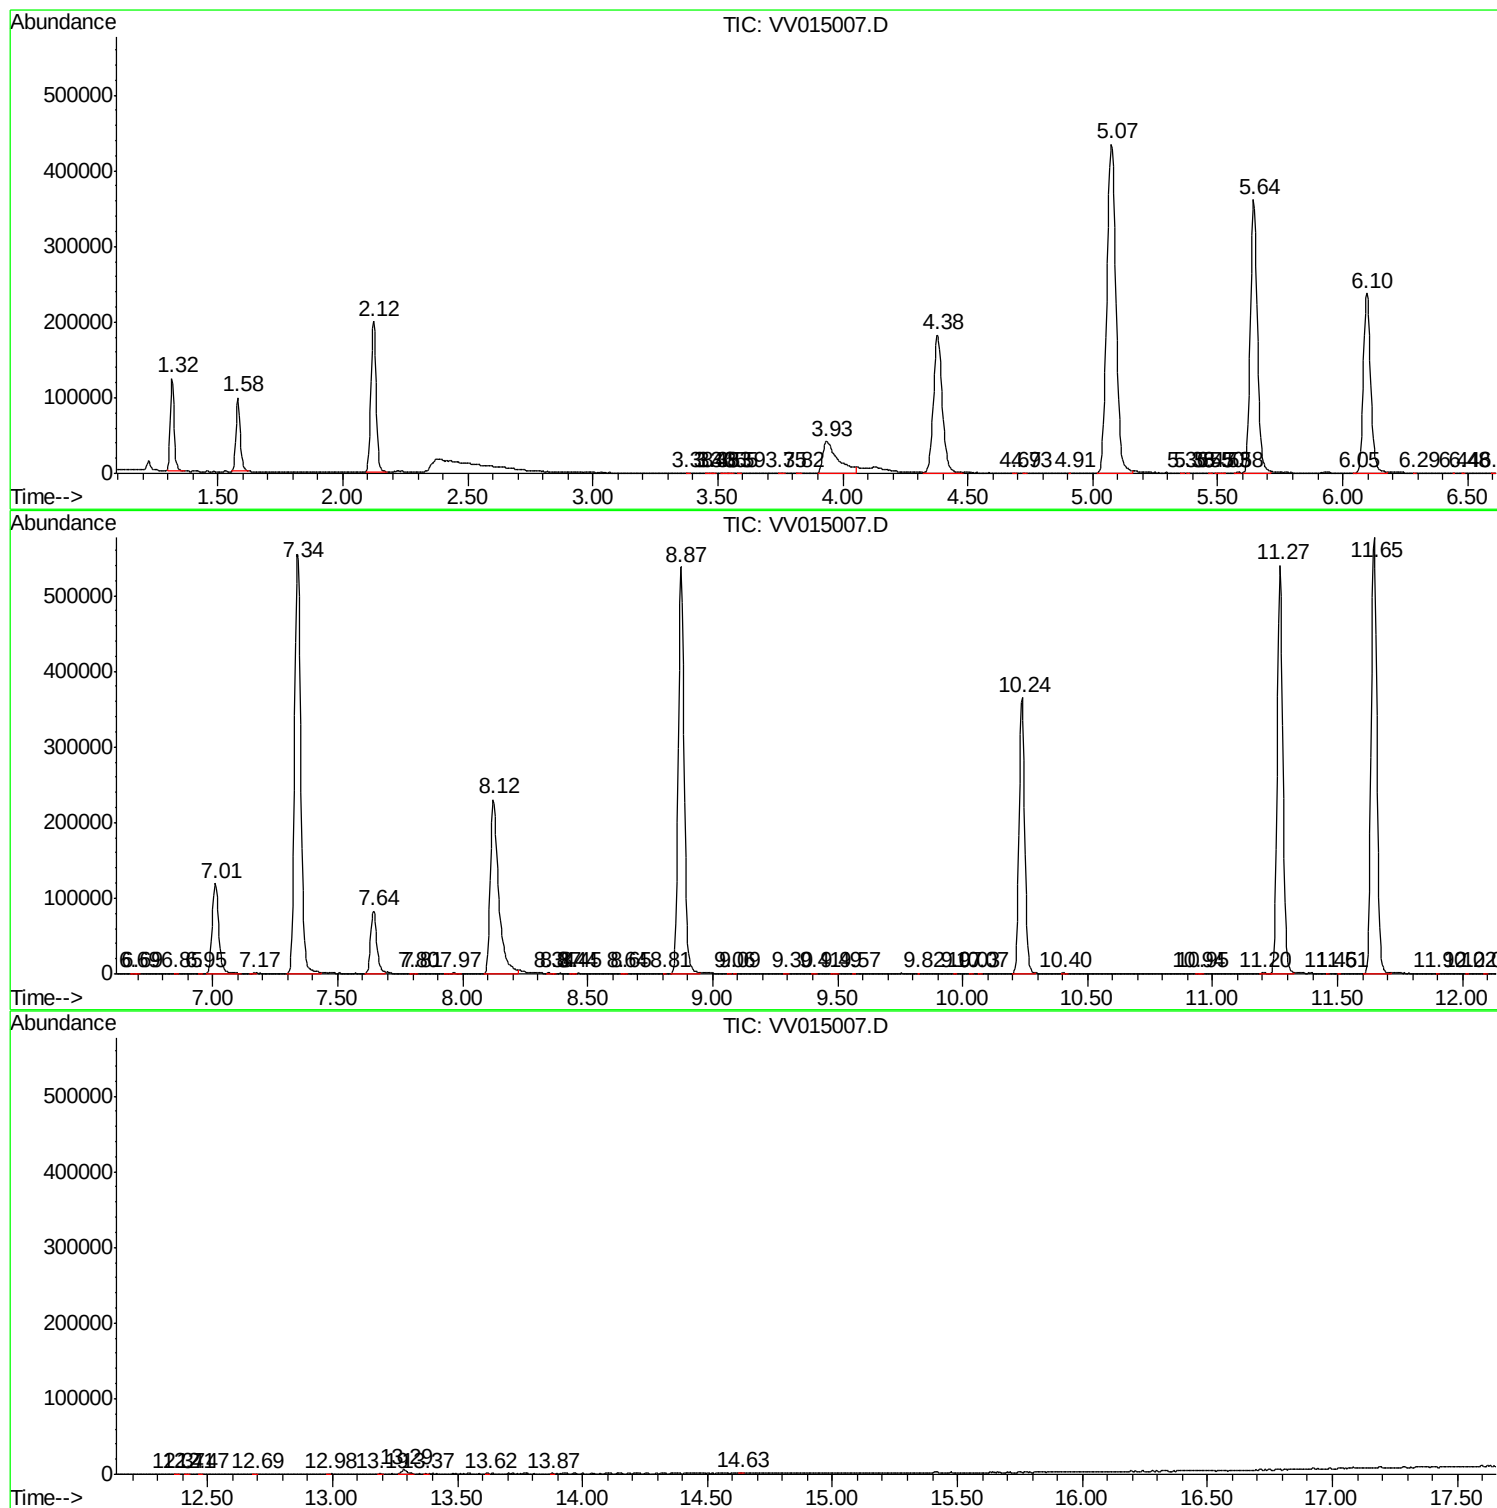

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015007.D
Acq On : 18 Mar 2020 05:12
Operator : SY/MD
Sample : L1940-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D89

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015007.D
Acq On : 18 Mar 2020 05:12
Operator : SY/MD
Sample : L1940-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D89

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc