

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015008.D
 Acq On : 18 Mar 2020 05:36
 Operator : SY/MD
 Sample : L1940-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	89	rVB	129822	133433	12.25%	1.591%
2	1.579	145	152	169	rVB	95471	116569	10.70%	1.390%
3	2.122	311	321	335	rBV	198281	285766	26.23%	3.407%
4	2.923	566	570	574	rBV2	458	337	0.03%	0.004%
5	3.003	592	595	598	rBV	207	115	0.01%	0.001%
6	3.187	647	652	655	rBV4	472	382	0.04%	0.005%
7	3.454	732	735	738	rBV	192	145	0.01%	0.002%
8	3.534	756	760	761	rBV	177	97	0.01%	0.001%
9	3.743	823	825	827	rBV	191	121	0.01%	0.001%
10	3.826	849	851	853	rBV	178	83	0.01%	0.001%
11	3.852	856	859	862	rBV2	343	243	0.02%	0.003%
12	3.881	866	868	871	rVB2	234	123	0.01%	0.001%
13	3.933	873	884	915	rBV2	41520	169287	15.54%	2.018%
14	4.380	1008	1023	1044	rBV2	174614	434852	39.92%	5.184%
15	4.679	1114	1116	1118	rBV	287	169	0.02%	0.002%
16	4.781	1147	1148	1151	rVB2	278	126	0.01%	0.002%
17	4.807	1151	1156	1158	rBV2	350	353	0.03%	0.004%
18	5.074	1221	1239	1264	rBV2	431603	1089258	100.00%	12.985%
19	5.312	1309	1313	1316	rBV2	596	497	0.05%	0.006%
20	5.363	1326	1329	1331	rBV2	497	296	0.03%	0.004%
21	5.412	1342	1344	1346	rBV2	328	184	0.02%	0.002%
22	5.470	1358	1362	1365	rBV2	249	243	0.02%	0.003%
23	5.486	1365	1367	1371	rVB2	346	247	0.02%	0.003%
24	5.643	1401	1416	1446	rBV	351549	696000	63.90%	8.297%
25	5.904	1494	1497	1498	rBV2	265	148	0.01%	0.002%
26	5.923	1499	1503	1504	rBV2	689	502	0.05%	0.006%
27	5.968	1514	1517	1519	rBV2	526	407	0.04%	0.005%
28	6.016	1530	1532	1534	rBV	260	93	0.01%	0.001%
29	6.096	1543	1557	1588	rBV	238785	484481	44.48%	5.775%
30	6.206	1588	1591	1593	rBV2	639	347	0.03%	0.004%
31	6.370	1640	1642	1644	rVB2	299	112	0.01%	0.001%
32	6.514	1684	1687	1690	rBV2	305	229	0.02%	0.003%
33	6.595	1707	1712	1715	rBV	315	411	0.04%	0.005%
34	6.717	1747	1750	1753	rBV	231	195	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015008.D
 Acq On : 18 Mar 2020 05:36
 Operator : SY/MD
 Sample : L1940-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.785	1769	1771	1774	rVB2	242	105	0.01%	0.001%
36	6.887	1801	1803	1804	rBV2	155	46	0.00%	0.001%
37	7.010	1829	1841	1857	rBV	117043	210595	19.33%	2.510%
38	7.277	1921	1924	1926	rBV2	373	204	0.02%	0.002%
39	7.338	1930	1943	1965	rBV	546302	941328	86.42%	11.221%
40	7.585	2018	2020	2022	rVB	403	146	0.01%	0.002%
41	7.643	2025	2038	2054	rBV	83548	143916	13.21%	1.716%
42	7.775	2076	2079	2082	rBV3	229	218	0.02%	0.003%
43	7.804	2086	2088	2092	rBV2	221	167	0.02%	0.002%
44	7.826	2093	2095	2098	rVV2	214	81	0.01%	0.001%
45	8.122	2175	2187	2232	rBV3	233796	543680	49.91%	6.481%
46	8.383	2266	2268	2271	rBV2	343	205	0.02%	0.002%
47	8.598	2331	2335	2336	rBV	364	203	0.02%	0.002%
48	8.871	2407	2420	2445	rBV	531222	865592	79.47%	10.318%
49	9.087	2485	2487	2489	rVB	343	125	0.01%	0.001%
50	9.157	2507	2509	2510	rBV	375	179	0.02%	0.002%
51	9.283	2546	2548	2550	rBV	267	106	0.01%	0.001%
52	9.572	2636	2638	2640	rBV	378	178	0.02%	0.002%
53	9.701	2674	2678	2681	rBV2	377	275	0.03%	0.003%
54	9.749	2688	2693	2696	rBV	336	444	0.04%	0.005%
55	9.820	2711	2715	2722	rBV2	444	481	0.04%	0.006%
56	10.055	2786	2788	2794	rVB	374	330	0.03%	0.004%
57	10.083	2794	2797	2800	rBV	403	260	0.02%	0.003%
58	10.238	2833	2845	2864	rBV	355633	566599	52.02%	6.754%
59	10.556	2941	2944	2950	rBV2	478	330	0.03%	0.004%
60	10.675	2979	2981	2983	rBV	352	162	0.01%	0.002%
61	10.714	2991	2993	2995	rVB	268	92	0.01%	0.001%
62	10.781	3009	3014	3016	rBV2	279	296	0.03%	0.004%
63	10.868	3039	3041	3043	rBV	287	135	0.01%	0.002%
64	10.968	3069	3072	3073	rBV2	260	129	0.01%	0.002%
65	11.180	3136	3138	3141	rVB	350	147	0.01%	0.002%
66	11.199	3141	3144	3145	rBV	355	211	0.02%	0.003%
67	11.270	3154	3166	3188	rBV	514509	814839	74.81%	9.713%
68	11.450	3220	3222	3224	rVB	324	127	0.01%	0.002%
69	11.646	3270	3283	3305	rBV	551147	875359	80.36%	10.435%
70	11.826	3337	3339	3341	rBV2	246	80	0.01%	0.001%
71	12.067	3411	3414	3416	rBV	363	240	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015008.D
Acq On : 18 Mar 2020 05:36
Operator : SY/MD
Sample : L1940-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D90

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Title : VOC Analysis

72	12.093	3419	3422	3425	rBV2	366	255	0.02%	0.003%
73	12.177	3446	3448	3450	rBV	479	263	0.02%	0.003%
74	12.913	3674	3677	3679	rBV	418	230	0.02%	0.003%
75	13.186	3760	3762	3766	rBV2	504	307	0.03%	0.004%
76	13.283	3787	3792	3802	rBV5	2797	3758	0.35%	0.045%
77	13.823	3958	3960	3965	rBV2	540	519	0.05%	0.006%


Sum of corrected areas: 8388793

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015008.D
Acq On : 18 Mar 2020 05:36
Operator : SY/MD
Sample : L1940-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D90

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

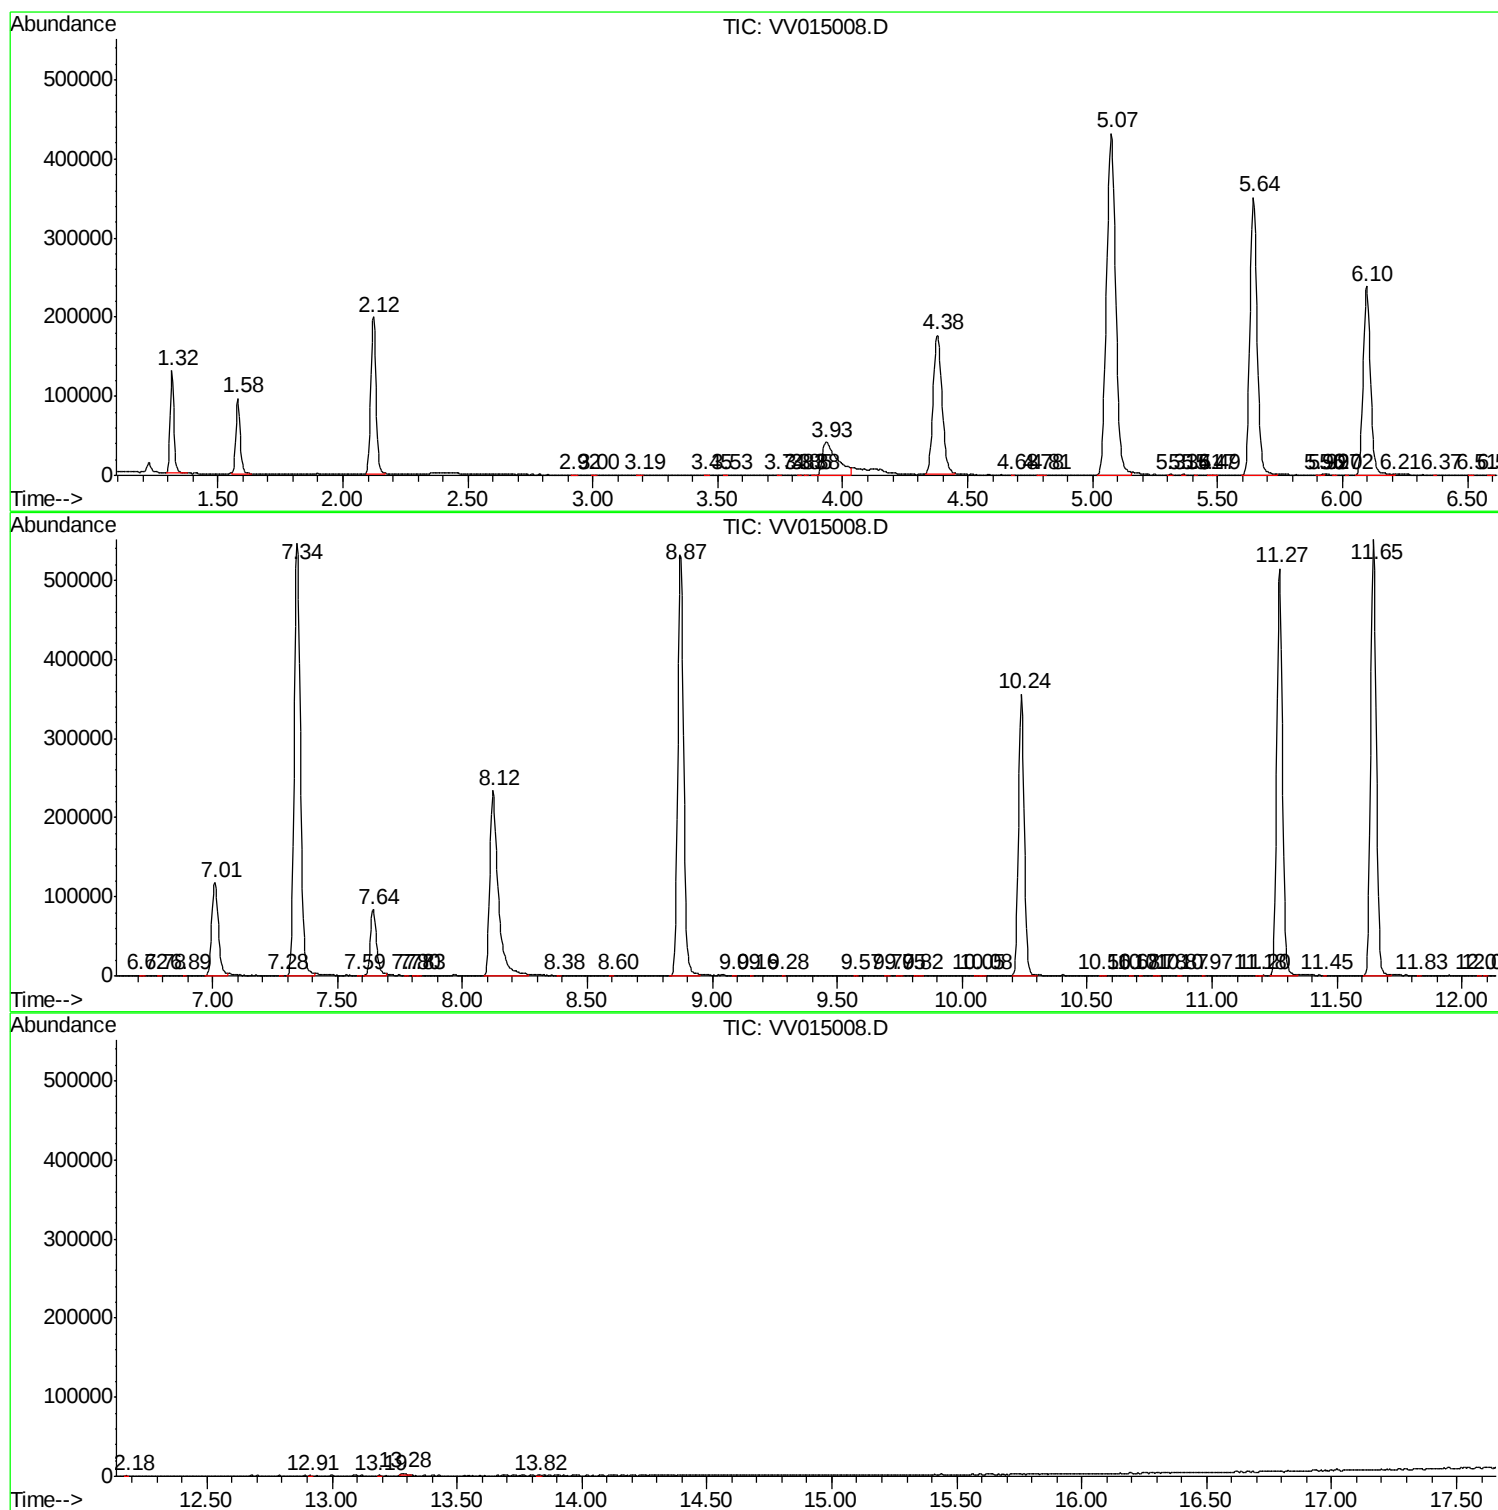

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015008.D
Acq On : 18 Mar 2020 05:36
Operator : SY/MD
Sample : L1940-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D90

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015008.D
Acq On : 18 Mar 2020 05:36
Operator : SY/MD
Sample : L1940-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D90

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc