

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015010.D
 Acq On : 18 Mar 2020 06:25
 Operator : SY/MD
 Sample : L1941-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	38	41	48	rVB3	12238	11009	0.02%	0.012%
2	1.315	64	70	90	rVB	114874	123306	0.23%	0.130%
3	1.579	145	152	171	rVB	88826	108792	0.21%	0.115%
4	2.122	312	321	337	rVB	190016	270939	0.51%	0.287%
5	2.878	553	556	557	rVB2	288	99	0.00%	0.000%
6	2.904	560	564	565	rBV2	375	294	0.00%	0.000%
7	2.968	582	584	587	rBV	274	163	0.00%	0.000%
8	2.991	589	591	593	rBV	312	151	0.00%	0.000%
9	3.042	604	607	610	rBV2	362	219	0.00%	0.000%
10	3.055	610	611	614	rBV	230	103	0.00%	0.000%
11	3.094	622	623	627	rVB	507	189	0.00%	0.000%
12	3.116	628	630	632	rBV	179	66	0.00%	0.000%
13	3.222	661	663	666	rBV2	168	89	0.00%	0.000%
14	3.261	672	675	680	rBV2	193	152	0.00%	0.000%
15	3.338	697	699	702	rBV	146	67	0.00%	0.000%
16	3.409	717	721	722	rBV2	263	200	0.00%	0.000%
17	3.479	740	743	744	rBV	143	86	0.00%	0.000%
18	3.511	750	753	755	rBV2	173	126	0.00%	0.000%
19	3.640	791	793	798	rBV2	269	190	0.00%	0.000%
20	3.775	831	835	837	rBV2	300	211	0.00%	0.000%
21	3.794	838	841	843	rBV2	373	246	0.00%	0.000%
22	3.929	872	883	908	rBV	40810	156240	0.30%	0.165%
23	4.380	1007	1023	1049	rBV2	177027	432068	0.82%	0.457%
24	4.595	1087	1090	1093	rBV	266	179	0.00%	0.000%
25	4.646	1104	1106	1108	rBV	208	89	0.00%	0.000%
26	4.672	1112	1114	1116	rVB	253	109	0.00%	0.000%
27	4.733	1130	1133	1142	rVB2	369	392	0.00%	0.000%
28	4.801	1152	1154	1158	rVB3	362	174	0.00%	0.000%
29	4.894	1182	1183	1185	rVB	113	28	0.00%	0.000%
30	4.917	1185	1190	1194	rBV2	420	434	0.00%	0.000%
31	4.965	1203	1205	1207	rBV	161	112	0.00%	0.000%
32	4.994	1211	1214	1218	rBV	147	168	0.00%	0.000%
33	5.074	1219	1239	1272	rBV2	423049	1083428	2.05%	1.146%
34	5.335	1317	1320	1324	rBV3	623	442	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015010.D
 Acq On : 18 Mar 2020 06:25
 Operator : SY/MD
 Sample : L1941-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	5.373	1330	1332	1334	rVB2	239	72	0.00%	0.000%
36	5.502	1369	1372	1375	rBV	425	319	0.00%	0.000%
37	5.544	1382	1385	1388	rBV2	213	105	0.00%	0.000%
38	5.643	1402	1416	1444	rBV	350182	693411	1.31%	0.734%
39	5.833	1470	1475	1478	rBV2	500	477	0.00%	0.001%
40	5.933	1499	1506	1507	rBV2	987	1010	0.00%	0.001%
41	5.997	1524	1526	1531	rBV2	413	283	0.00%	0.000%
42	6.032	1534	1537	1540	rBV2	292	228	0.00%	0.000%
43	6.097	1543	1557	1576	rBV	233442	475806	0.90%	0.503%
44	6.331	1628	1630	1632	rBV	229	106	0.00%	0.000%
45	6.376	1641	1644	1645	rBV	237	144	0.00%	0.000%
46	6.634	1722	1724	1727	rBV2	289	190	0.00%	0.000%
47	6.753	1757	1761	1763	rBV2	200	192	0.00%	0.000%
48	7.010	1827	1841	1859	rBV	118301	213500	0.40%	0.226%
49	7.235	1908	1911	1915	rBV2	383	283	0.00%	0.000%
50	7.338	1930	1943	1967	rBV	555568	949588	1.79%	1.005%
51	7.585	2018	2020	2023	rVB2	444	161	0.00%	0.000%
52	7.601	2023	2025	2027	rBV	236	146	0.00%	0.000%
53	7.643	2027	2038	2055	rBV2	82409	142782	0.27%	0.151%
54	7.929	2125	2127	2129	rVB2	264	93	0.00%	0.000%
55	7.942	2129	2131	2132	rBV	285	117	0.00%	0.000%
56	7.997	2144	2148	2155	rBV5	728	593	0.00%	0.001%
57	8.042	2159	2162	2163	rBV	209	127	0.00%	0.000%
58	8.119	2175	2186	2223	rBV	231624	525881	0.99%	0.556%
59	8.402	2270	2274	2275	rBV2	332	213	0.00%	0.000%
60	8.521	2309	2311	2317	rBV3	350	264	0.00%	0.000%
61	8.707	2367	2369	2373	rBV2	198	93	0.00%	0.000%
62	8.730	2374	2376	2380	rBV3	315	209	0.00%	0.000%
63	8.769	2385	2388	2394	rVB3	375	333	0.00%	0.000%
64	8.797	2394	2397	2399	rBV2	177	106	0.00%	0.000%
65	8.904	2406	2430	2470	rBV	8957314	15166789	28.66%	16.047%
66	9.267	2540	2543	2546	rBV2	661	536	0.00%	0.001%
67	9.611	2648	2650	2651	rBV	177	50	0.00%	0.000%
68	9.701	2676	2678	2679	rBV	173	52	0.00%	0.000%
69	9.791	2704	2706	2708	rBV	323	166	0.00%	0.000%
70	10.177	2825	2826	2827	rBV	165	50	0.00%	0.000%
71	10.186	2827	2829	2831	rVB2	315	91	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015010.D
 Acq On : 18 Mar 2020 06:25
 Operator : SY/MD
 Sample : L1941-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	10.238	2831	2845	2862	rBV	354546	564315	1.07%	0.597%
73	10.347	2875	2879	2882	rBV2	321	310	0.00%	0.000%
74	10.399	2891	2895	2898	rBV4	1005	996	0.00%	0.001%
75	10.444	2905	2909	2916	rBV3	1077	1388	0.00%	0.001%
76	10.498	2924	2926	2928	rBV	235	91	0.00%	0.000%
77	10.868	3039	3041	3042	rBV2	368	102	0.00%	0.000%
78	10.932	3056	3061	3063	rBV2	464	388	0.00%	0.000%
79	11.129	3120	3122	3125	rBV	206	85	0.00%	0.000%
80	11.199	3132	3144	3156	rBV	1013167	1541598	2.91%	1.631%
81	11.293	3156	3173	3197	rVB2	3709545	6493786	12.27%	6.871%
82	11.588	3264	3265	3266	rBV2	170	58	0.00%	0.000%
83	11.608	3267	3271	3272	rBV3	615	475	0.00%	0.001%
84	11.672	3272	3291	3310	rBV	31997502	52912507	100.00%	55.982%
85	12.135	3431	3435	3438	rBV3	1879	1431	0.00%	0.002%
86	12.418	3513	3523	3536	rBV2	50439	78224	0.15%	0.083%
87	12.495	3545	3547	3552	rVB3	570	363	0.00%	0.000%
88	12.601	3569	3580	3591	rVV5	8230	18432	0.03%	0.020%
89	12.669	3594	3601	3609	rVB6	4649	6481	0.01%	0.007%
90	12.768	3624	3632	3645	rVB3	21234	32178	0.06%	0.034%
91	13.055	3720	3721	3722	rBV	353	99	0.00%	0.000%
92	13.170	3754	3757	3763	rVB3	426	465	0.00%	0.000%
93	13.283	3778	3792	3819	rBV	7029489	10630401	20.09%	11.247%
94	13.765	3929	3942	3961	rBV	1129755	1732504	3.27%	1.833%
95	14.842	4264	4277	4292	rVB	50902	83870	0.16%	0.089%
96	15.418	4449	4456	4467	rVB2	35550	50755	0.10%	0.054%


Sum of corrected areas: 94516428

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015010.D
Acq On : 18 Mar 2020 06:25
Operator : SY/MD
Sample : L1941-11
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

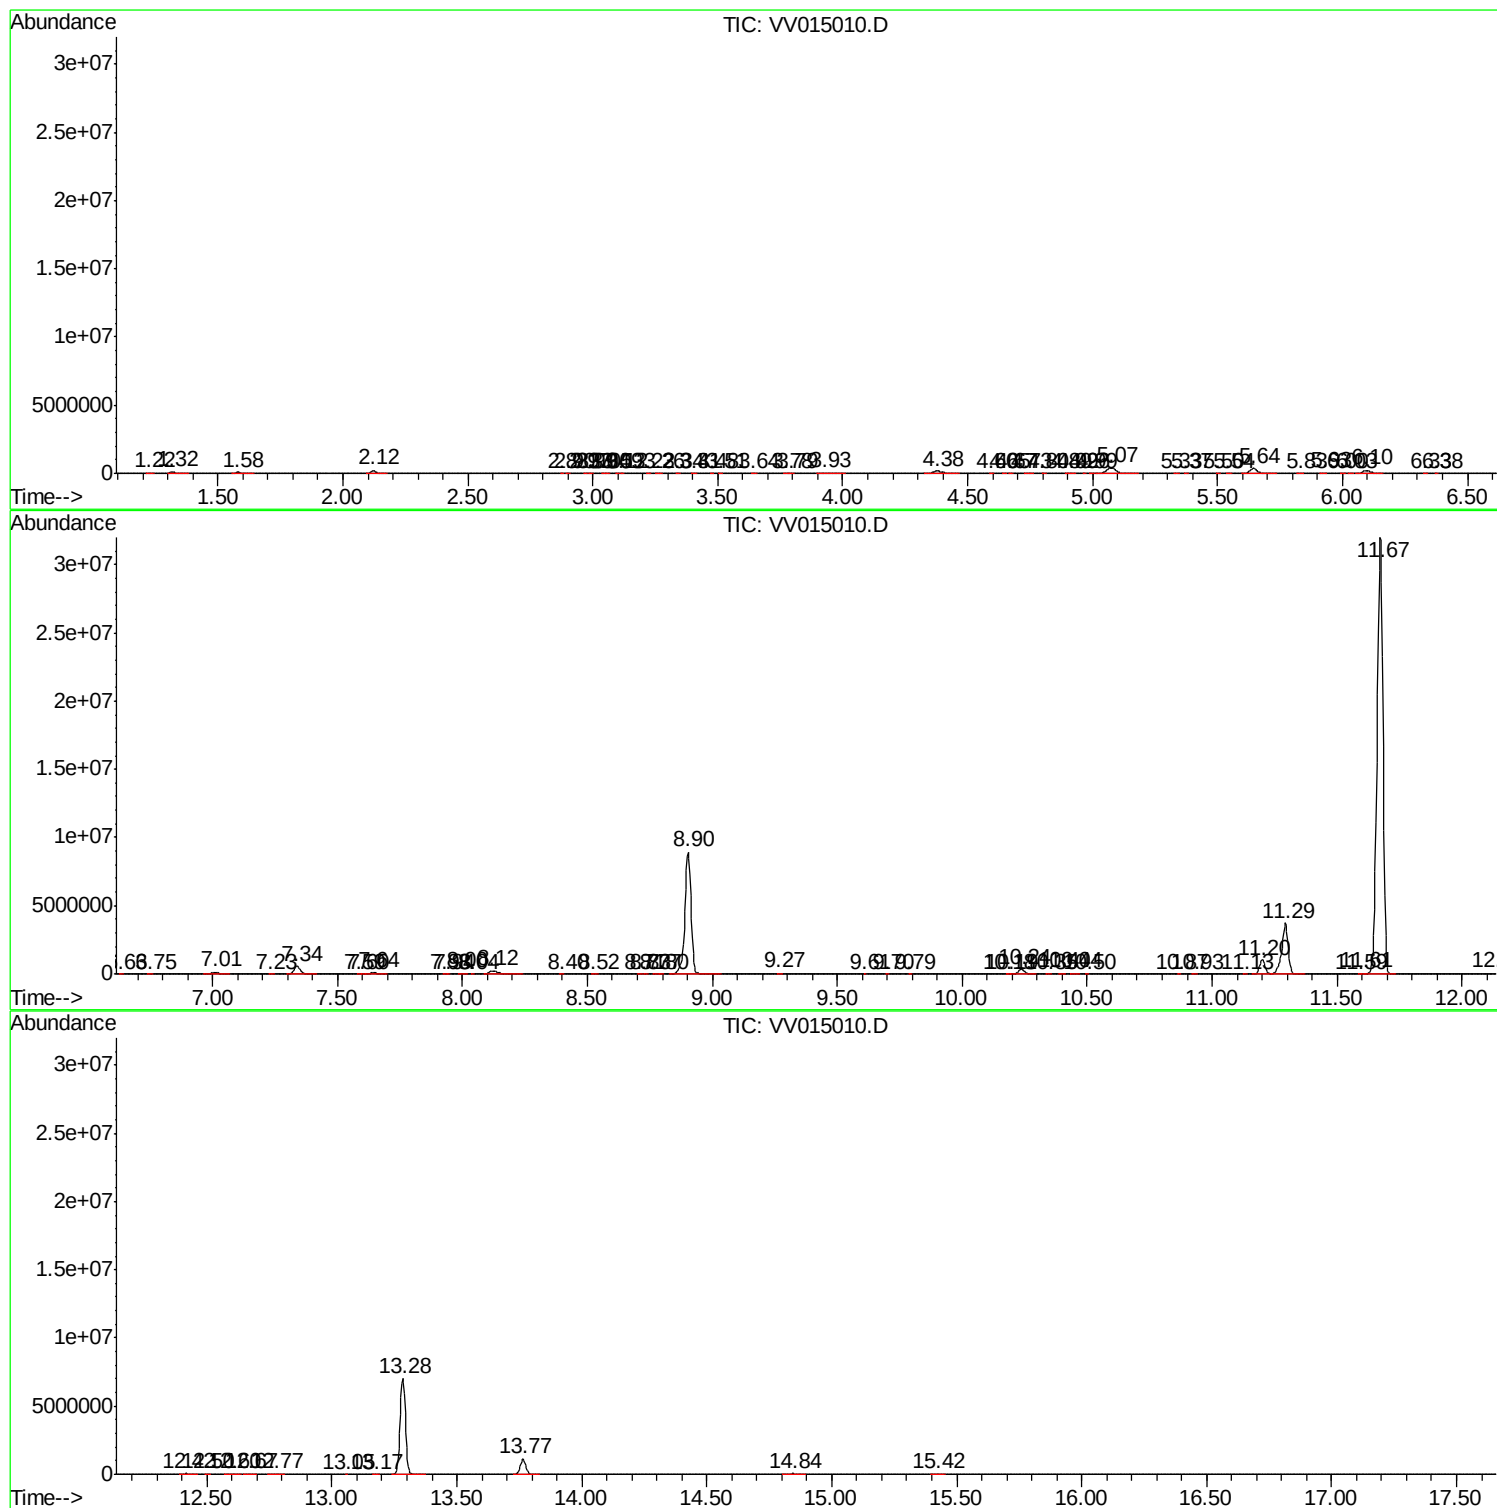

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015010.D
Acq On : 18 Mar 2020 06:25
Operator : SY/MD
Sample : L1941-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015010.D
Acq On : 18 Mar 2020 06:25
Operator : SY/MD
Sample : L1941-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc