

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015011.D
 Acq On : 18 Mar 2020 06:49
 Operator : SY/MD
 Sample : L1941-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	37	41	48	rVB4	11127	10875	0.01%	0.008%
2	1.315	63	70	90	rVB	115969	125583	0.17%	0.094%
3	1.579	144	152	172	rVB	88744	111823	0.15%	0.083%
4	1.669	176	180	182	rBV3	803	619	0.00%	0.000%
5	1.724	195	197	202	rVB2	1031	613	0.00%	0.000%
6	2.122	310	321	337	rVB	187173	270239	0.36%	0.202%
7	2.193	340	343	345	rBV2	969	758	0.00%	0.001%
8	2.302	373	377	378	rBV2	1161	748	0.00%	0.001%
9	2.871	552	554	557	rBV2	391	228	0.00%	0.000%
10	3.077	614	618	623	rBV3	388	278	0.00%	0.000%
11	3.164	640	645	647	rVB	495	392	0.00%	0.000%
12	3.187	647	652	654	rBV3	354	299	0.00%	0.000%
13	3.515	750	754	756	rBV2	284	220	0.00%	0.000%
14	3.762	828	831	833	rBV	682	473	0.00%	0.000%
15	3.781	833	837	838	rVV	427	348	0.00%	0.000%
16	3.933	871	884	919	rBV	40900	168337	0.22%	0.126%
17	4.379	1006	1023	1049	rBV	171519	427829	0.57%	0.319%
18	4.653	1104	1108	1109	rBV2	441	298	0.00%	0.000%
19	4.785	1146	1149	1153	rVB3	292	208	0.00%	0.000%
20	4.971	1204	1207	1213	rVB2	325	250	0.00%	0.000%
21	5.003	1213	1217	1220	rBV2	326	259	0.00%	0.000%
22	5.074	1221	1239	1253	rBV2	425068	1083104	1.44%	0.808%
23	5.289	1302	1306	1309	rBV	520	386	0.00%	0.000%
24	5.325	1315	1317	1322	rBV2	596	413	0.00%	0.000%
25	5.376	1330	1333	1337	rVB2	407	269	0.00%	0.000%
26	5.441	1350	1353	1356	rBV2	275	212	0.00%	0.000%
27	5.643	1402	1416	1441	rBV2	345751	684922	0.91%	0.511%
28	5.785	1453	1460	1463	rBV3	476	526	0.00%	0.000%
29	5.810	1466	1468	1476	rVB3	447	280	0.00%	0.000%
30	5.920	1499	1502	1503	rBV2	762	445	0.00%	0.000%
31	6.096	1543	1557	1580	rBV	228809	472070	0.63%	0.352%
32	6.228	1594	1598	1601	rBV4	969	694	0.00%	0.001%
33	6.289	1615	1617	1622	rVB	486	302	0.00%	0.000%
34	6.344	1630	1634	1638	rVB2	449	325	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015011.D
 Acq On : 18 Mar 2020 06:49
 Operator : SY/MD
 Sample : L1941-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

35	6.646	1724	1728	1731	rBV3	325	272	0.00%	0.000%
36	7.010	1828	1841	1865	rBV	117044	211219	0.28%	0.158%
37	7.096	1866	1868	1871	rVB3	518	286	0.00%	0.000%
38	7.174	1888	1892	1897	rVV3	735	580	0.00%	0.000%
39	7.338	1929	1943	1965	rBV	548808	943447	1.25%	0.704%
40	7.457	1977	1980	1985	rVB3	430	310	0.00%	0.000%
41	7.518	1997	1999	2003	rVB3	405	224	0.00%	0.000%
42	7.563	2008	2013	2020	rBV4	541	863	0.00%	0.001%
43	7.643	2027	2038	2059	rBV	80630	140346	0.19%	0.105%
44	7.823	2090	2094	2098	rBV2	284	243	0.00%	0.000%
45	7.920	2119	2124	2126	rBV2	285	226	0.00%	0.000%
46	7.952	2129	2134	2135	rBV	411	352	0.00%	0.000%
47	8.122	2174	2187	2226	rBV2	218750	534125	0.71%	0.399%
48	8.325	2249	2250	2255	rBV2	448	338	0.00%	0.000%
49	8.411	2275	2277	2281	rVB2	452	264	0.00%	0.000%
50	8.672	2355	2358	2361	rBV	259	235	0.00%	0.000%
51	8.903	2409	2430	2471	rBV	13772534	22831180	30.32%	17.041%
52	9.138	2500	2503	2507	rBV3	682	577	0.00%	0.000%
53	9.447	2596	2599	2606	rVB3	523	629	0.00%	0.000%
54	9.608	2647	2649	2652	rVB2	537	218	0.00%	0.000%
55	9.932	2747	2750	2753	rBV	321	214	0.00%	0.000%
56	9.981	2763	2765	2771	rVB	301	210	0.00%	0.000%
57	10.006	2771	2773	2778	rVB	495	253	0.00%	0.000%
58	10.035	2778	2782	2785	rBV2	277	300	0.00%	0.000%
59	10.238	2832	2845	2861	rBV	355542	562388	0.75%	0.420%
60	10.331	2871	2874	2877	rBV3	310	220	0.00%	0.000%
61	10.402	2893	2896	2904	rVV4	951	1149	0.00%	0.001%
62	10.450	2904	2911	2918	rVB3	1458	1953	0.00%	0.001%
63	10.550	2940	2942	2943	rBV	507	250	0.00%	0.000%
64	10.778	3010	3013	3016	rBV	367	221	0.00%	0.000%
65	11.042	3091	3095	3097	rBV2	259	223	0.00%	0.000%
66	11.202	3132	3145	3156	rBV	1547761	2378965	3.16%	1.776%
67	11.292	3156	3173	3198	rVB	5666570	9438924	12.54%	7.045%
68	11.559	3253	3256	3259	rVB3	1155	667	0.00%	0.000%
69	11.678	3271	3293	3310	rBV2	42967179	75297884	100.00%	56.203%
70	12.058	3408	3411	3414	rBV3	703	589	0.00%	0.000%
71	12.125	3429	3432	3433	rBV	972	526	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031720\
 Data File : VV015011.D
 Acq On : 18 Mar 2020 06:49
 Operator : SY/MD
 Sample : L1941-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis

72	12.193	3450	3453	3455	rBV2	438	289	0.00%	0.000%
73	12.260	3472	3474	3480	rBV3	644	613	0.00%	0.000%
74	12.289	3480	3483	3487	rBV5	634	491	0.00%	0.000%
75	12.337	3496	3498	3499	rBV2	582	260	0.00%	0.000%
76	12.357	3502	3504	3511	rVB5	1771	1988	0.00%	0.001%
77	12.418	3512	3523	3535	rBV	80214	123744	0.16%	0.092%
78	12.601	3569	3580	3593	rVV3	12792	31300	0.04%	0.023%
79	12.665	3593	3600	3610	rVB3	7135	11083	0.01%	0.008%
80	12.768	3620	3632	3647	rVV2	32297	50911	0.07%	0.038%
81	12.826	3648	3650	3653	rVB2	576	307	0.00%	0.000%
82	13.016	3704	3709	3712	rBV3	1995	2088	0.00%	0.002%
83	13.051	3718	3720	3727	rVB4	528	476	0.00%	0.000%
84	13.135	3743	3746	3750	rVB3	425	302	0.00%	0.000%
85	13.154	3750	3752	3755	rBV	409	270	0.00%	0.000%
86	13.286	3774	3793	3815	rBV	10207879	15370156	20.41%	11.472%
87	13.431	3835	3838	3844	rBV5	1162	1440	0.00%	0.001%
88	13.524	3861	3867	3875	rVB4	5797	7542	0.01%	0.006%
89	13.765	3927	3942	3967	rBV	1632781	2453347	3.26%	1.831%
90	14.074	4035	4038	4042	rBV2	512	347	0.00%	0.000%
91	14.096	4042	4045	4046	rBV2	652	317	0.00%	0.000%
92	14.212	4076	4081	4085	rBV4	446	533	0.00%	0.000%
93	14.231	4085	4087	4090	rVB2	735	369	0.00%	0.000%
94	14.295	4104	4107	4108	rBV2	472	273	0.00%	0.000%
95	14.312	4110	4112	4113	rBV2	776	305	0.00%	0.000%
96	14.414	4142	4144	4146	rBV	412	216	0.00%	0.000%
97	14.530	4178	4180	4183	rVB2	1138	632	0.00%	0.000%
98	14.842	4261	4277	4292	rBV2	66901	113551	0.15%	0.085%
99	15.266	4407	4409	4415	rVB3	733	530	0.00%	0.000%
100	15.418	4446	4456	4470	rBV	55040	86696	0.12%	0.065%


Sum of corrected areas: 133975871

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031720\
Data File : VV015011.D
Acq On : 18 Mar 2020 06:49
Operator : SY/MD
Sample : L1941-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

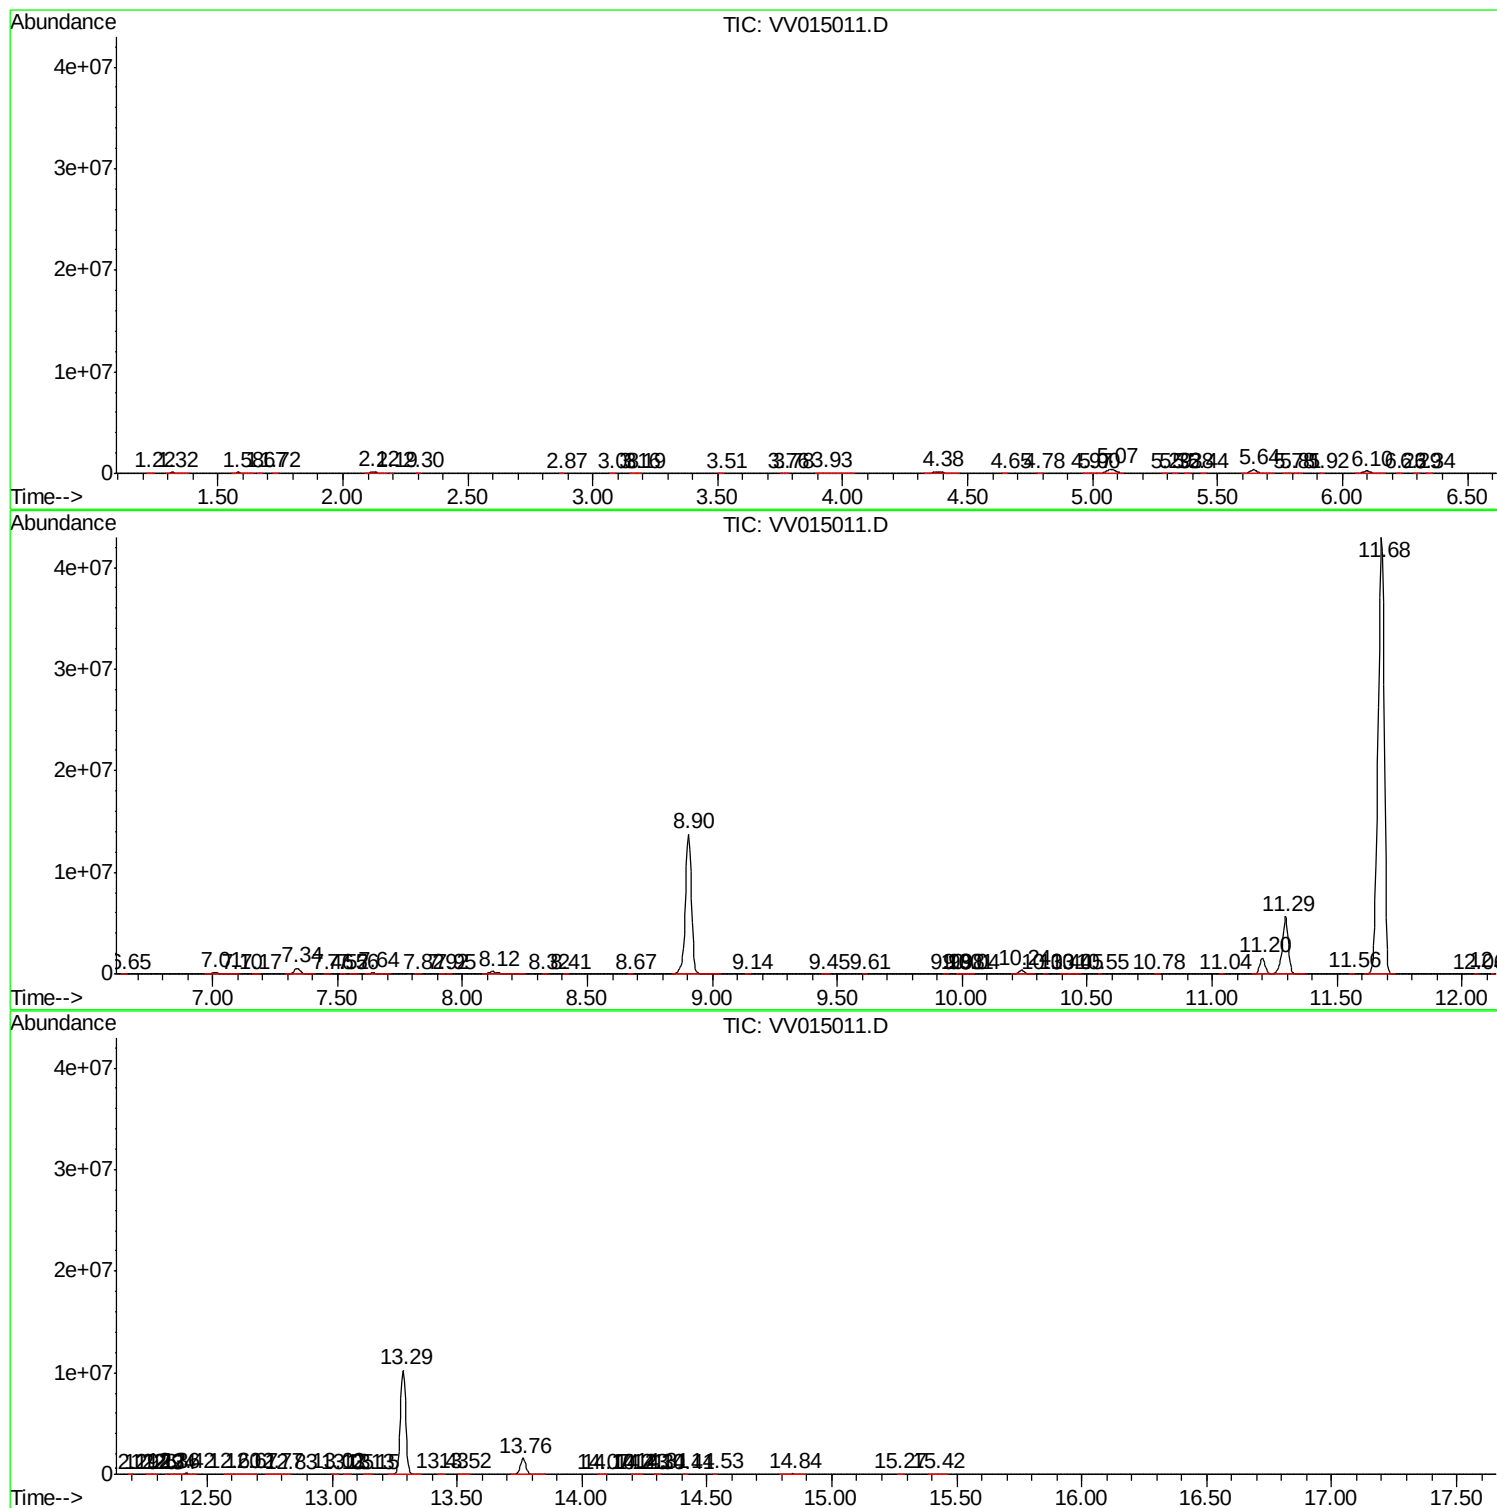

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015011.D
Acq On : 18 Mar 2020 06:49
Operator : SY/MD
Sample : L1941-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031720\
Data File : VV015011.D
Acq On : 18 Mar 2020 06:49
Operator : SY/MD
Sample : L1941-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc