


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031720\
 Data File : VV014964.D
 Acq On : 17 Mar 2020 10:23
 Operator : SY/MD
 Sample : BFB65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031620WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 18 13:06:03 2020

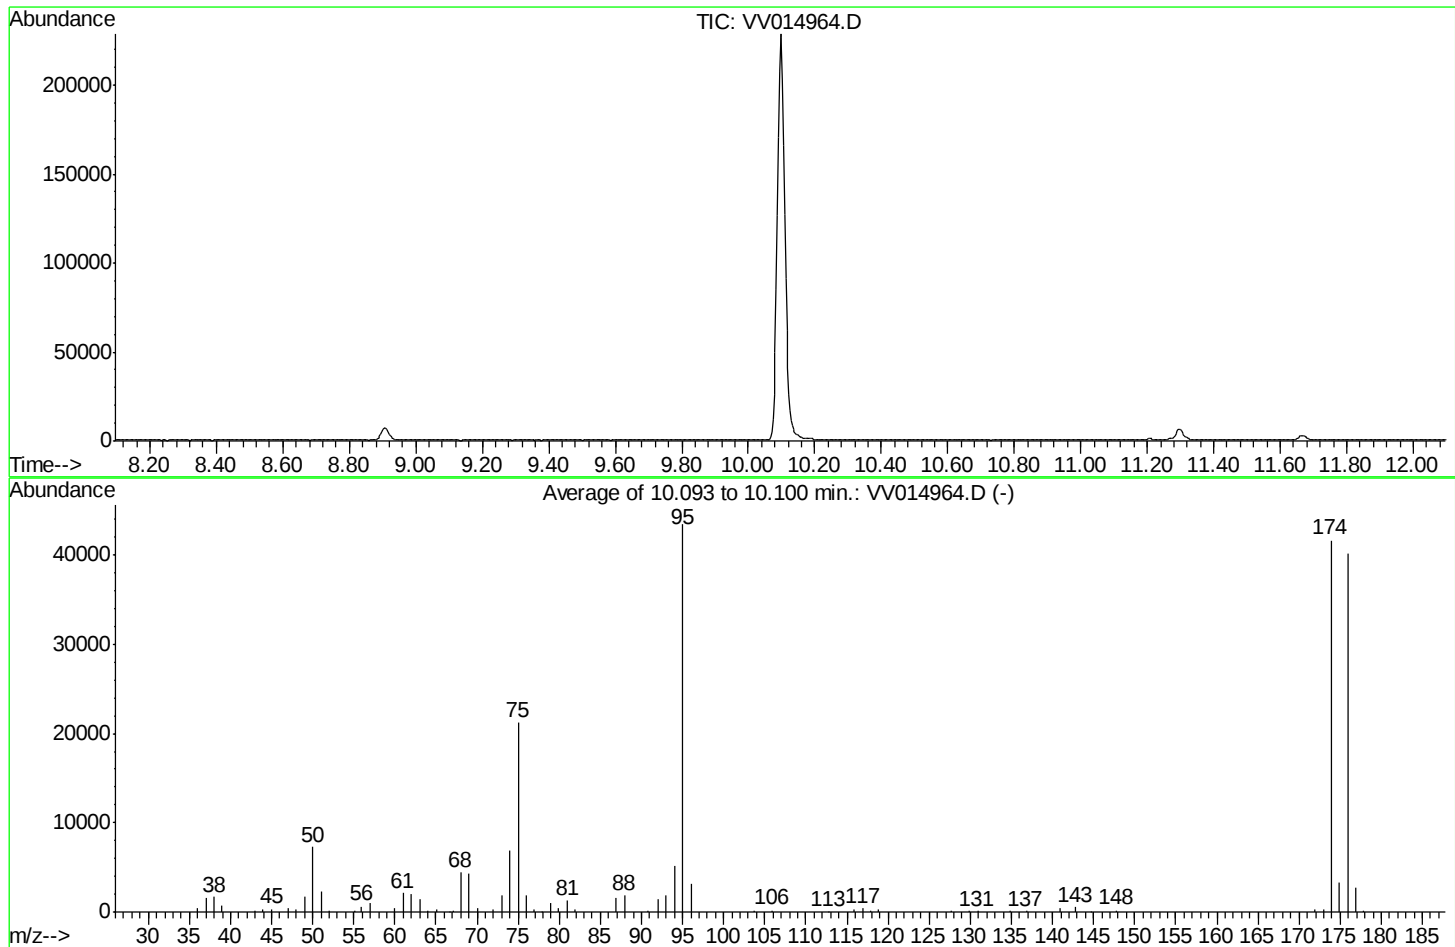

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	7272	PASS
75	95	30	80	48.8	21176	PASS
95	95	100	100	100.0	43434	PASS
96	95	5	9	7.4	3195	PASS
173	174	0.00	2	0.8	353	PASS
174	95	50	120	95.8	41594	PASS
175	174	5	9	7.8	3249	PASS
176	174	95	101	96.7	40226	PASS
177	176	5	9	6.6	2667	PASS

m/z	Abundance
36.00	373.0
37.00	1565.0
38.00	1566.0
38.90	652.0
40.00	189.0
43.00	117.0
43.90	430.0
45.00	333.0
47.00	535.0
48.00	248.0
49.00	1468.0
50.00	6763.0
51.00	2098.0
52.10	177.0
55.20	165.0
56.00	647.0
57.00	925.0
60.00	375.0
61.00	2003.0
62.00	1869.0
63.00	1398.0
64.00	201.0
65.10	226.0
67.10	107.0
68.00	4198.0
69.00	4255.0
70.00	344.0
72.00	291.0
73.00	1873.0
74.00	6853.0
75.00	20368.0
76.00	1862.0
77.00	352.0
78.90	985.0
79.90	410.0
81.00	1132.0
81.90	197.0
86.90	1485.0
88.00	1731.0
90.80	165.0
92.00	1258.0
93.00	1775.0
94.00	4914.0
95.00	40872.0
96.00	2922.0
103.70	159.0
105.90	217.0
115.80	212.0
117.00	377.0
117.90	119.0
118.80	230.0
127.80	175.0
130.90	110.0
140.80	413.0
142.90	554.0
147.90	134.0
171.90	247.0
173.00	353.0
173.90	38944.0
174.90	2891.0
175.90	37056.0
176.90	2727.0
177.80	142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	384.0
37.00	1682.0
38.00	1710.0
38.90	728.0
39.90	257.0
43.00	139.0
43.90	503.0
45.00	378.0
47.00	518.0
48.00	249.0
49.00	1717.0
50.00	7540.0
51.00	2324.0
52.10	160.0
55.10	147.0
56.00	644.0
57.00	996.0
59.90	428.0
61.00	2238.0
62.00	2100.0
63.00	1496.0
64.00	204.0
65.10	344.0
67.20	159.0
68.00	4621.0
69.00	4487.0
70.00	383.0
72.00	306.0
73.00	1952.0
74.00	7043.0
75.00	21760.0
76.00	1874.0
76.90	274.0
78.90	1058.0
79.90	411.0
81.00	1300.0
81.90	210.0
86.90	1698.0
87.90	1866.0
90.80	212.0
92.00	1454.0
93.00	1988.0
94.00	5428.0
95.00	44856.0
96.00	3324.0
103.80	136.0
105.90	187.0
112.80	106.0
115.90	297.0
116.90	412.0
117.90	174.0
118.80	273.0
127.70	106.0
129.80	134.0
130.90	145.0
134.80	125.0
136.80	143.0
140.80	472.0
142.80	616.0
144.70	117.0
147.80	160.0
171.90	300.0
173.00	372.0
173.90	42992.0
174.90	3328.0
175.90	41776.0
176.90	2753.0
177.80	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	387.0
37.00	1661.0
38.00	1695.0
39.00	622.0
39.90	306.0
43.90	552.0
45.00	350.0
47.10	431.0
48.00	244.0
49.00	1840.0
50.00	7514.0
51.00	2361.0
52.00	137.0
55.10	120.0
55.90	539.0
57.00	973.0
59.90	401.0
61.00	2153.0
62.00	1964.0
63.00	1449.0
64.00	175.0
65.10	414.0
66.70	102.0
67.20	186.0
68.00	4394.0
69.00	4191.0
70.10	420.0
72.00	309.0
73.00	1924.0
74.00	6656.0
75.00	21400.0
76.00	1788.0
76.80	260.0
77.80	110.0
78.90	1065.0
79.90	405.0
81.00	1290.0
81.90	297.0
86.90	1676.0
87.90	1828.0
90.80	193.0
92.00	1478.0
93.00	2005.0
94.00	5298.0
95.00	44576.0
96.00	3339.0
103.80	124.0
105.90	147.0
115.90	304.0
116.90	432.0
117.90	230.0
118.90	301.0
129.80	169.0
131.00	119.0
134.80	154.0
136.80	172.0
140.90	498.0
142.80	538.0
144.60	116.0
147.80	158.0
171.90	321.0
172.90	334.0
173.90	42848.0
174.90	3530.0
175.90	41848.0
176.90	2523.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Scan 2789 (10.058 min): VV014964.D
BFB65

m/z	Abundance
39.80	250.0
44.00	244.0
125.30	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65