


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031721\
Data File : VW020650.D
Acq On : 17 Mar 2021 13:17
Operator : SY/MD
Sample : M1675-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF7

Manual Integrations
APPROVED

MMDadoda
3/19/2021 11:27:50 AM

Quant Time: Mar 18 01:15:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 18 01:14:23 2021
Response via : Initial Calibration

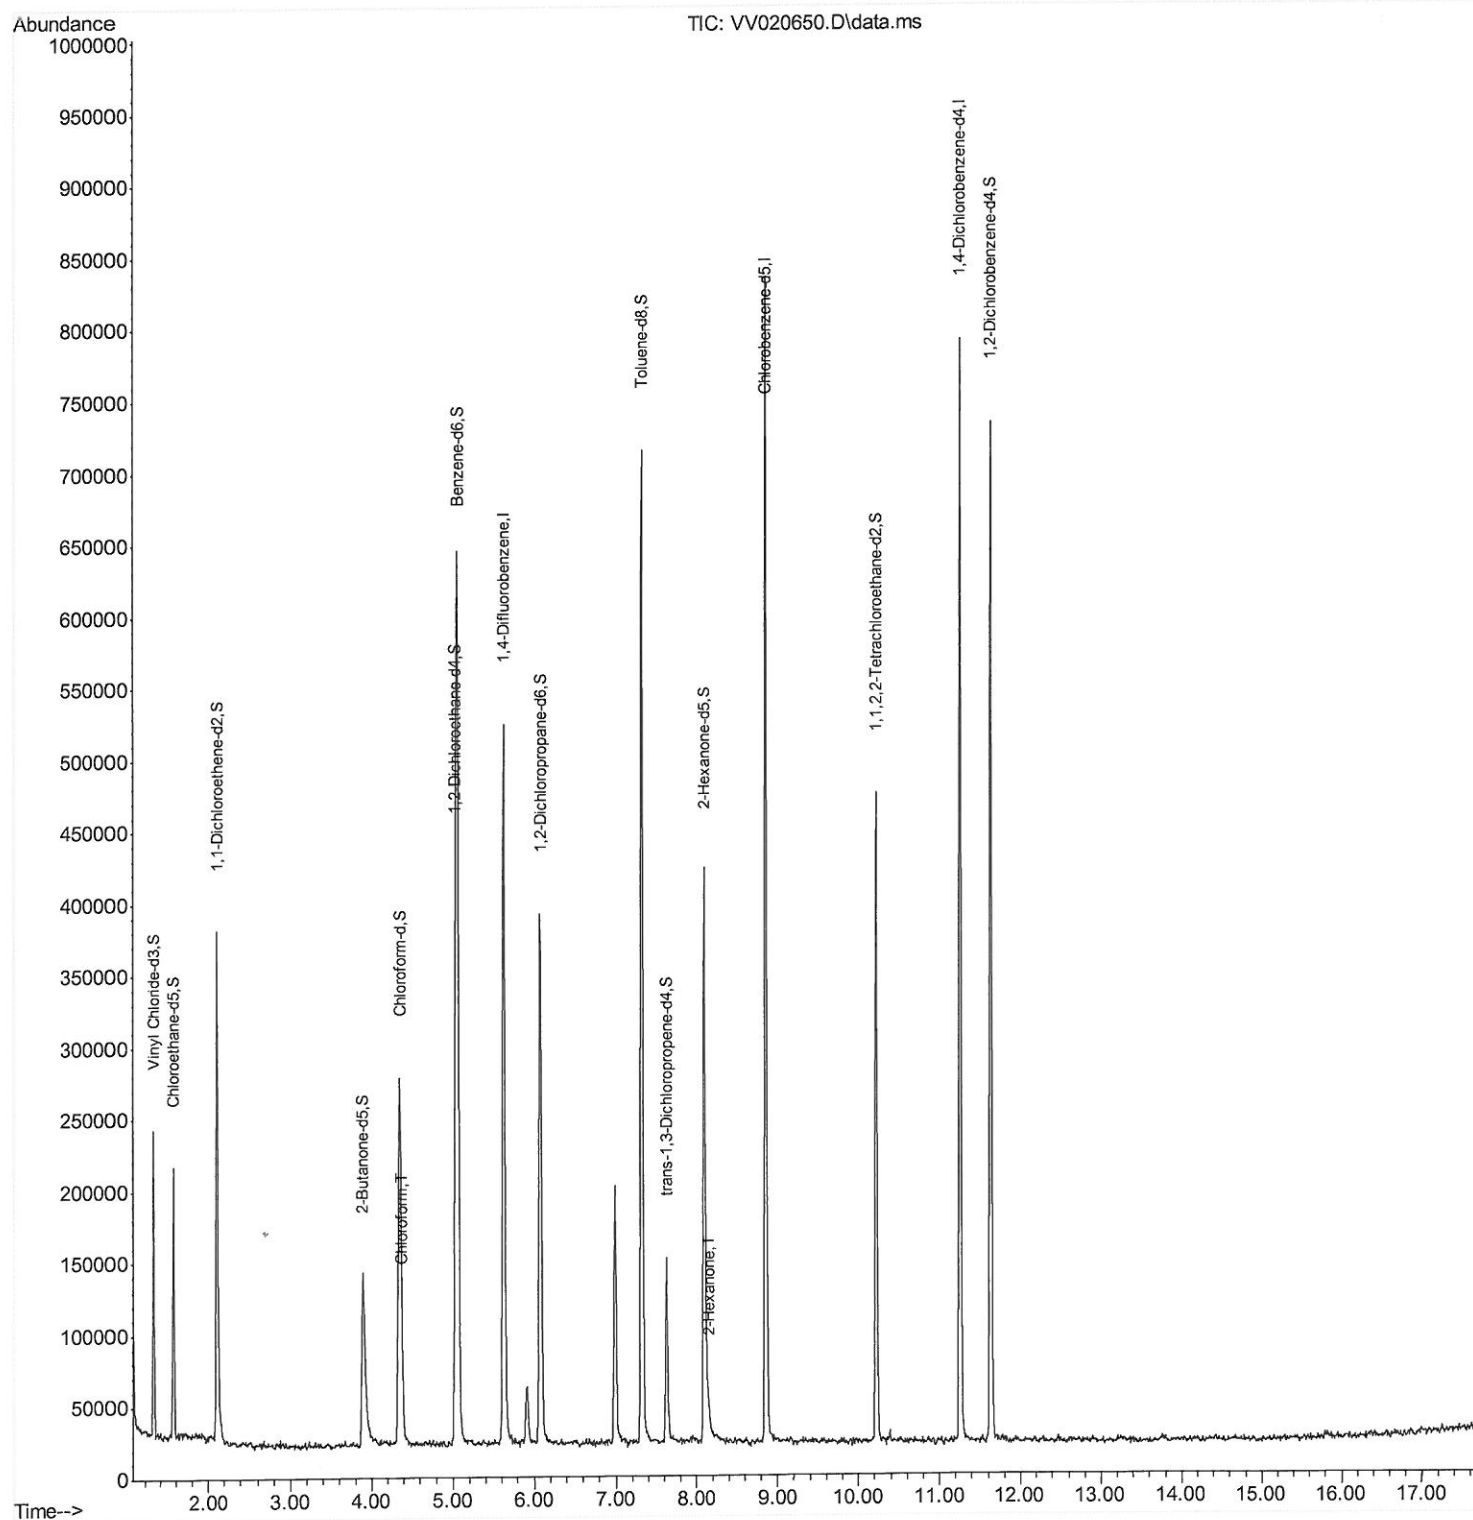

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031721\
Data File : VV020650.D
Acq On : 17 Mar 2021 13:17
Operator : SY/MD
Sample : M1675-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF7

Manual Integrations
APPROVED

MMDadoda
3/19/2021 11:27:50 AM

Quant Time: Mar 18 01:15:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 18 01:14:23 2021
Response via : Initial Calibration

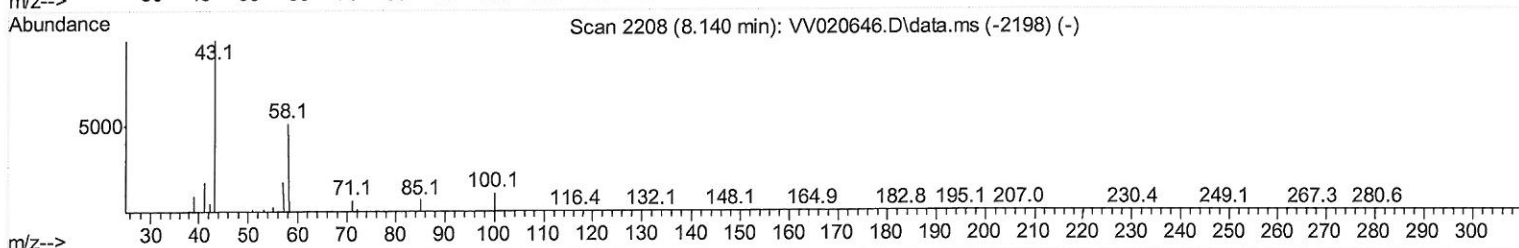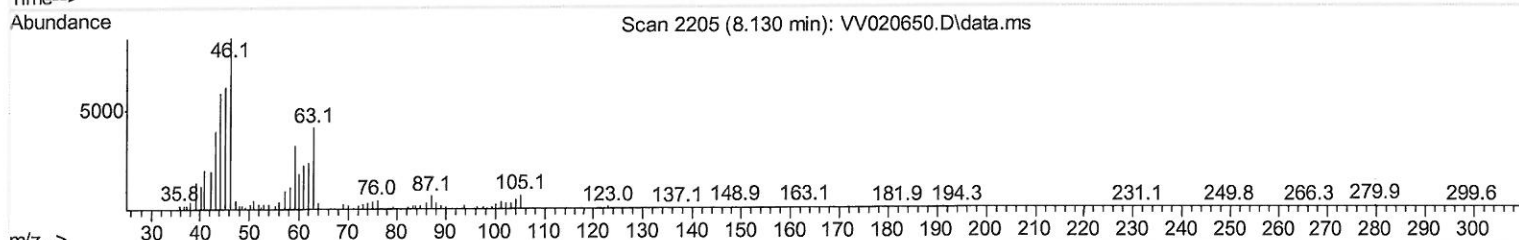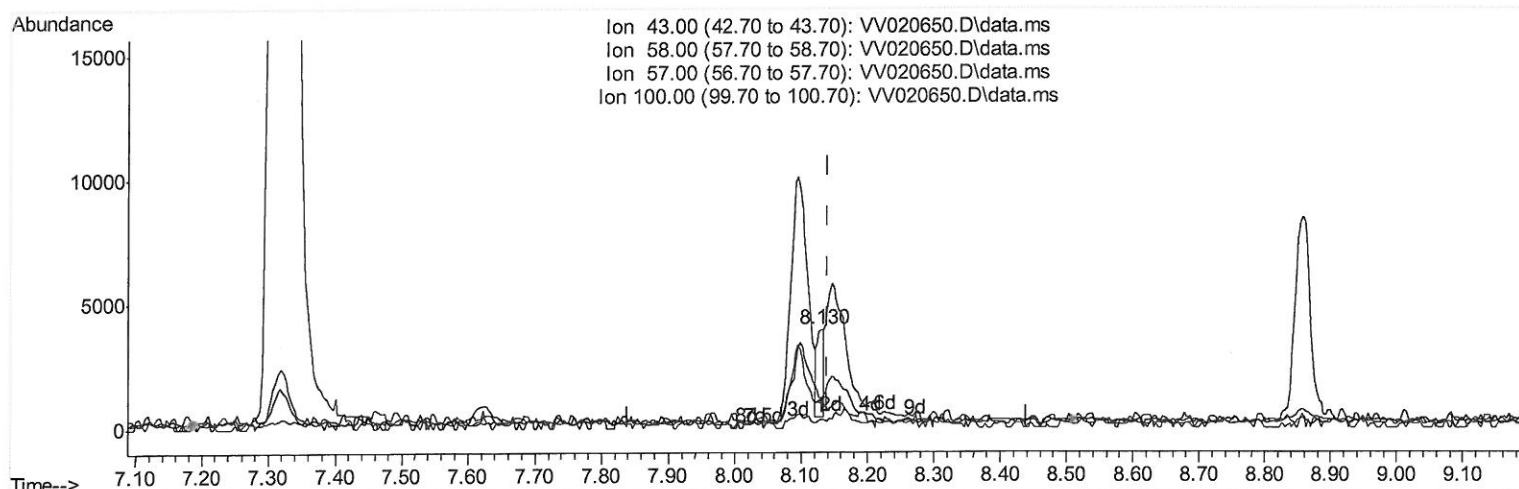

TIC: VV020650.D\data.ms

(48) 2-Hexanone (T)

8.130min (-0.010) 0.69 ug/L

response 2608

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	52.20	0.00#
57.00	18.70	0.00#
100.00	11.10	4.95#

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031721\
 Data File : VV020650.D
 Acq On : 17 Mar 2021 13:17
 Operator : SY/MD
 Sample : M1675-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0BF7

Manual Integrations
 APPROVED

MMDadoda
 3/19/2021 11:27:50 AM

Quant Time: Mar 18 01:15:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 18 01:14:23 2021
 Response via : Initial Calibration

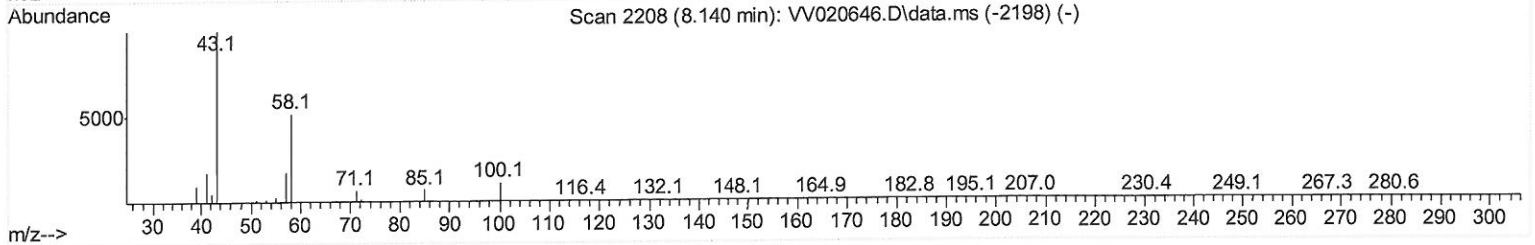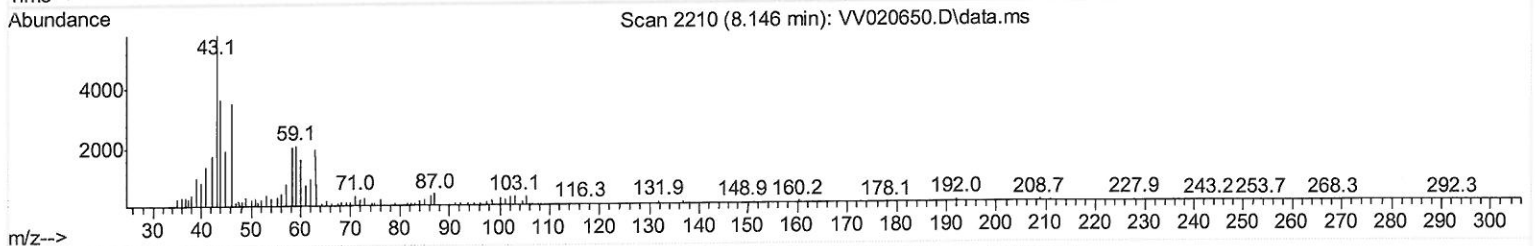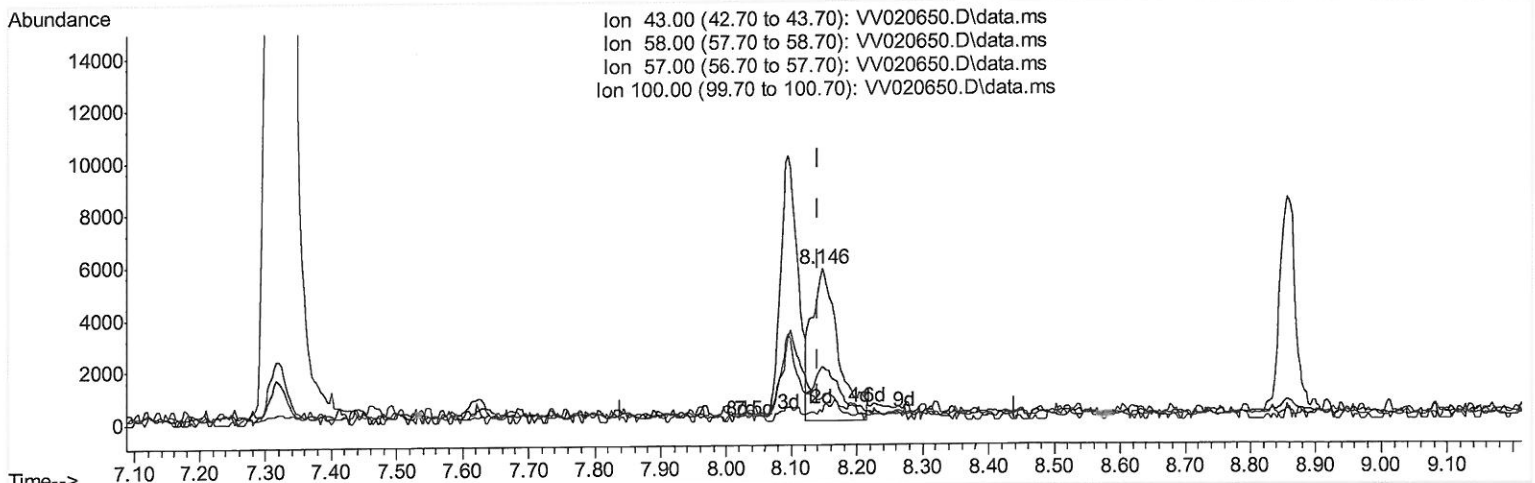

TIC: VV020650.D\data.ms

(48) 2-Hexanone (T)

8.146min (+ 0.006) 4.31 ug/L m

response 16258

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	52.20	0.00#
57.00	18.70	0.00#
100.00	11.10	0.79#

Handwritten: 7 MD
 3/19/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031721\
 Data File : VW020650.D
 Acq On : 17 Mar 2021 13:17
 Operator : SY/MD
 Sample : M1675-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF7

Manual Integrations
 APPROVED

MMDadoda
 3/19/2021 11:27:50 AM

Quant Time: Mar 18 01:15:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 18 01:14:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	419413	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	407545	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	180752	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	126990	37.54	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	75.08%		
7) Chloroethane-d5	1.571	69	110806	40.94	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	81.88%		
11) 1,1-Dichloroethene-d2	2.108	63	189267	29.43	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	58.86%#		
21) 2-Butanone-d5	3.895	46	230512	106.16	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	106.16%		
24) Chloroform-d	4.352	84	255103	43.38	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	86.76%		
26) 1,2-Dichloroethane-d4	5.034	65	175219	45.16	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	90.32%		
32) Benzene-d6	5.053	84	511550	45.43	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	90.86%		
36) 1,2-Dichloropropane-d6	6.072	67	171066	47.48	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	94.96%		
41) Toluene-d8	7.320	98	429367	42.90	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	85.80%		
43) trans-1,3-Dichloroprop...	7.625	79	69915	41.52	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	83.04%		
47) 2-Hexanone-d5	8.091	63	131146	97.30	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	97.30%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	206437	45.85	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	91.70%		
64) 1,2-Dichlorobenzene-d4	11.631	152	168339	48.06	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	96.12%		
Target Compounds						
25) Chloroform	4.381	83	21054	3.49	ug/L	95
48) 2-Hexanone	8.146	43	16258m	4.31	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 m0
 3/19/21