

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031721\
 Data File : VW020656.D
 Acq On : 17 Mar 2021 15:41
 Operator : SY/MD
 Sample : M1685-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG509

Manual Integrations
 APPROVED

MMDadoda
 3/19/2021 11:28:25 AM

Quant Time: Mar 18 01:17:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 18 01:14:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	418565	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	412450	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	180444	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	125145	37.07	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	74.14%	
7) Chloroethane-d5	1.571	69	107182	39.68	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.36%	
11) 1,1-Dichloroethene-d2	2.108	63	190562m	29.69	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	59.38%#	
21) 2-Butanone-d5	3.895	46	217133	100.20	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	100.20%	
24) Chloroform-d	4.352	84	253303	43.16	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	86.32%	
26) 1,2-Dichloroethane-d4	5.037	65	180496	46.61	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.22%	
32) Benzene-d6	5.053	84	500941	43.96	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.92%	
36) 1,2-Dichloropropane-d6	6.072	67	166198	45.58	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	91.16%	
41) Toluene-d8	7.320	98	429369	42.39	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	84.78%	
43) trans-1,3-Dichloroprop...	7.625	79	70432	41.33	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.66%	
47) 2-Hexanone-d5	8.095	63	118144	86.61	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	86.61%	
57) 1,1,2,2-Tetrachloroeth...	10.220	84	191229	41.97	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	83.94%	
64) 1,2-Dichlorobenzene-d4	11.631	152	163954	46.89	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.78%	
Target Compounds						
					Qvalue	
13) Acetone	2.191	43	11733m	6.63	ug/L	
25) Chloroform	4.384	83	11792	1.96	ug/L	94
48) 2-Hexanone	8.149	43	14525	3.81	ug/L #	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031721\
Data File : VV020656.D
Acq On : 17 Mar 2021 15:41
Operator : SY/MD
Sample : M1685-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
BG509

Manual Integrations
APPROVED

MMDadoda
3/19/2021 11:28:25 AM


Quant Time: Mar 18 01:17:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 18 01:14:23 2021
Response via : Initial Calibration

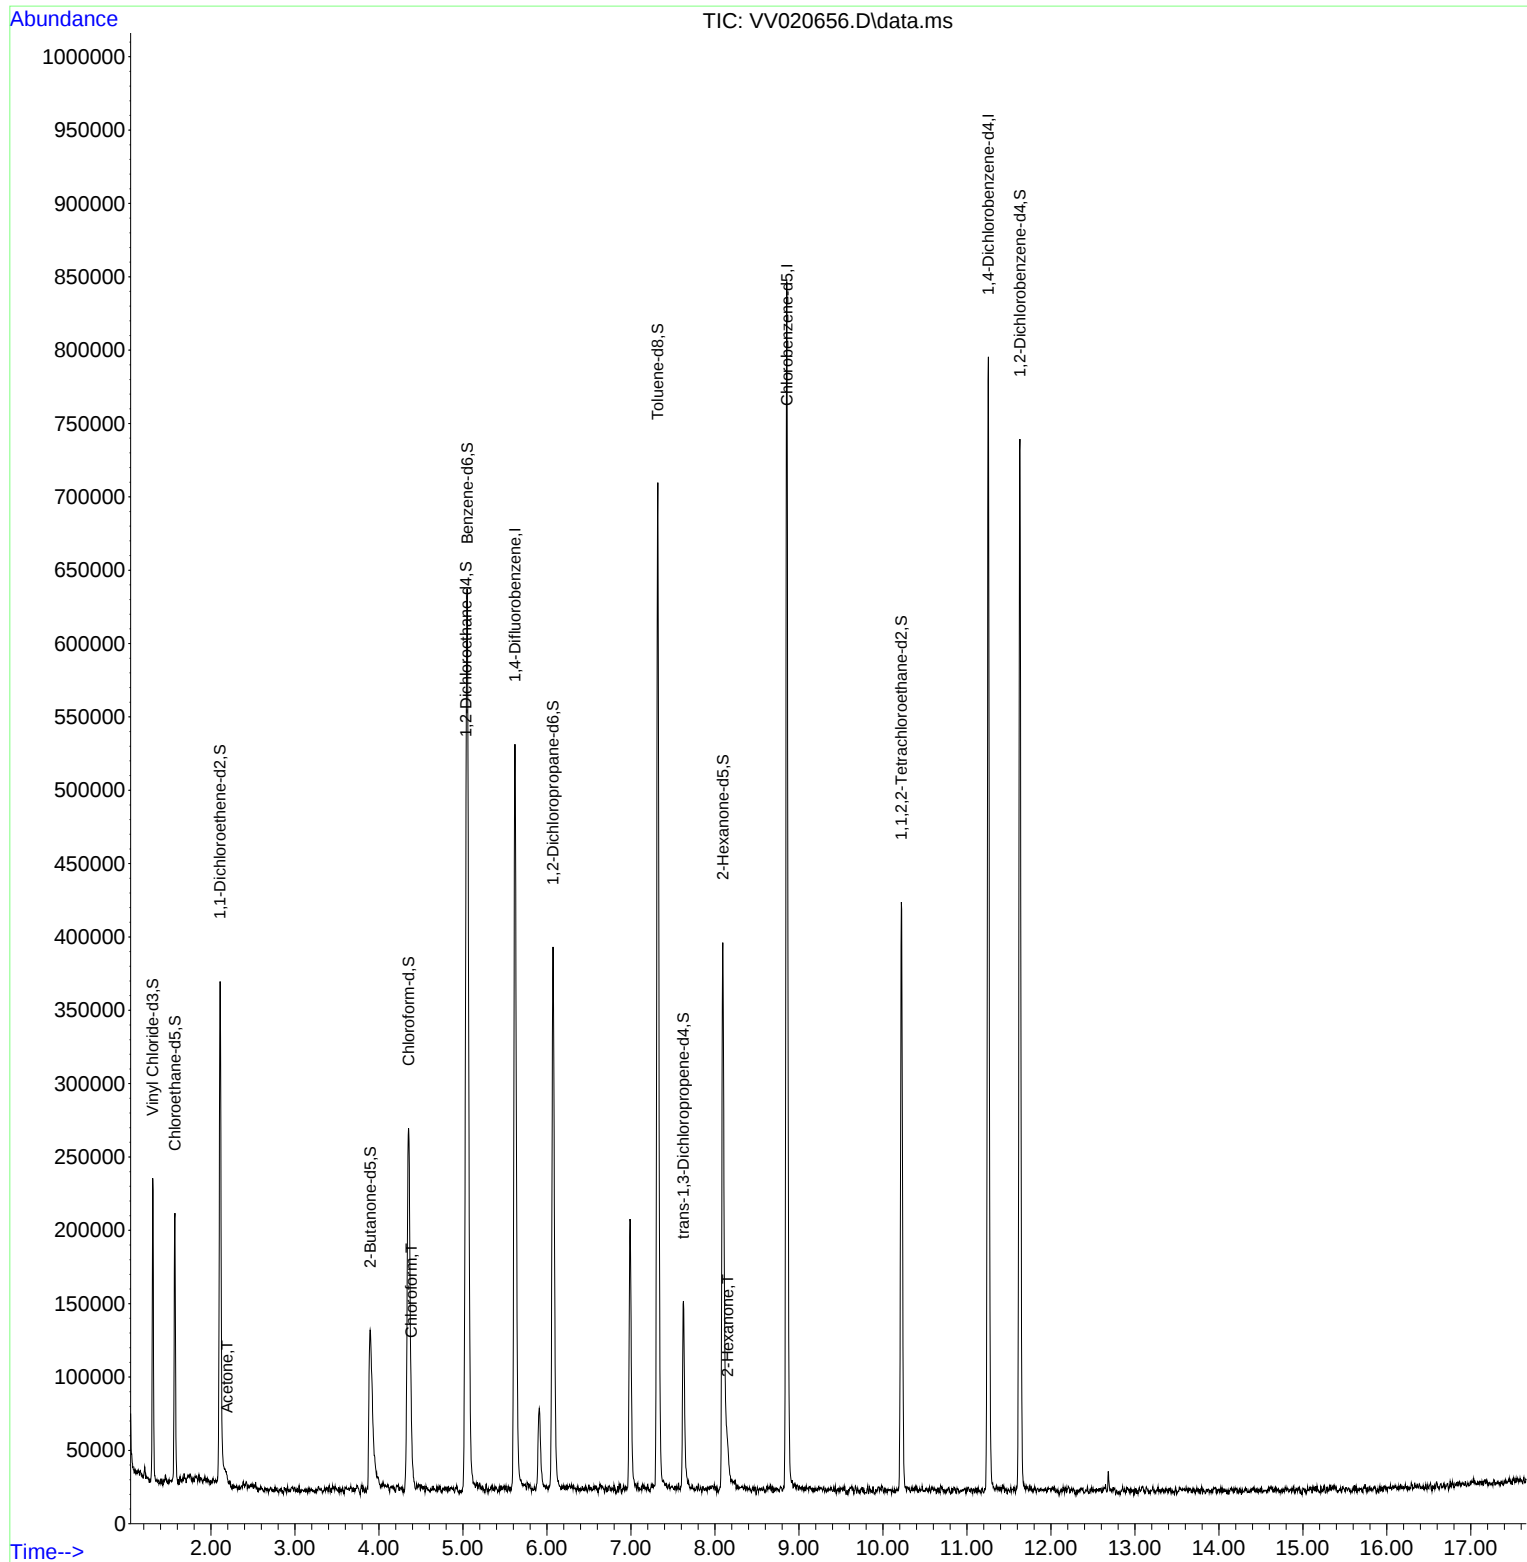

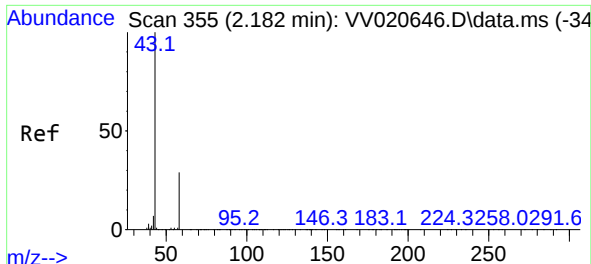

#13
Acetone
Concen: 6.63 ug/L m
RT: 2.191 min Scan# 358
Delta R.T. 0.009 min
Lab File: VV020656.D
Acq: 17 Mar 2021 15:41




Instrument :
MSVOA_V
ClientSampleId :
BG509

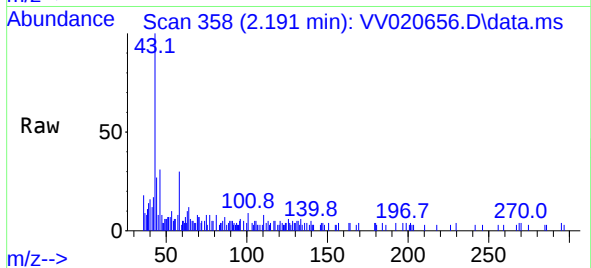


Tgt Ion: 43 Resp: 11733
Ion Ratio Lower Upper
43 100
58 14.6 0.0 60.2

Manual Integrations
APPROVED



MMDadoda
3/19/2021 11:28:25 AM

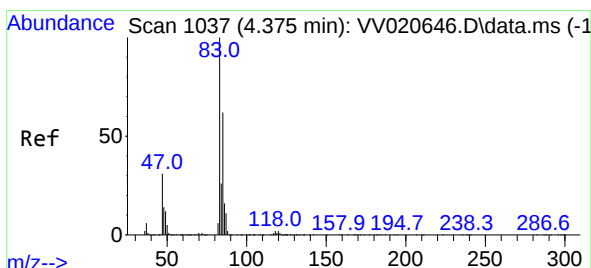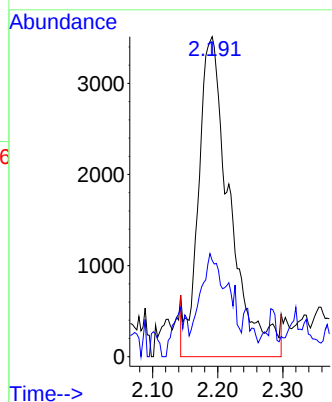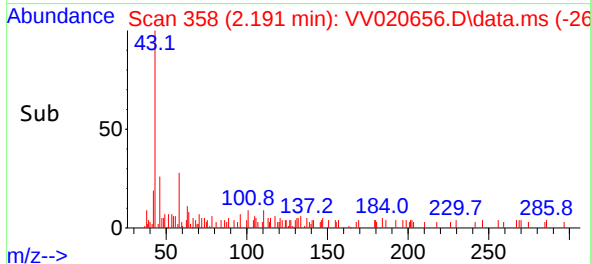


#25
Chloroform
Concen: 1.96 ug/L
RT: 4.384 min Scan# 1040
Delta R.T. 0.009 min
Lab File: VV020656.D
Acq: 17 Mar 2021 15:41

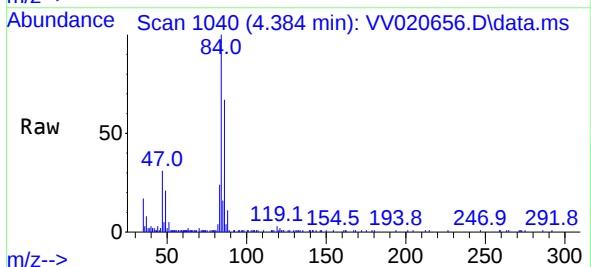

Tgt Ion: 83 Resp: 11792
Ion Ratio Lower Upper
83 100
85 67.9 44.2 82.2

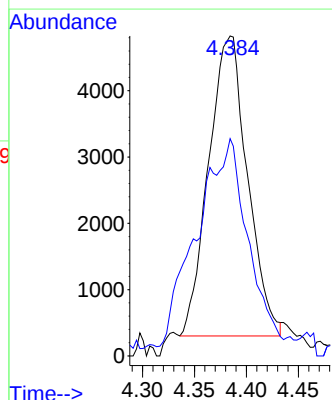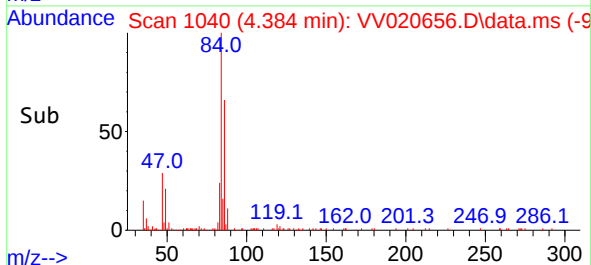

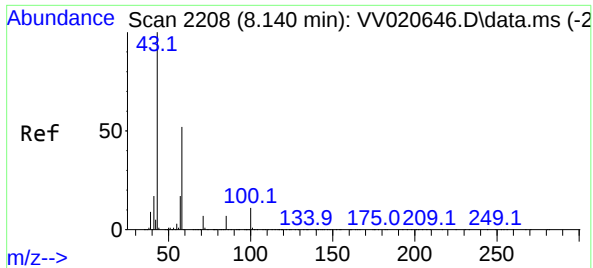

#48
2-Hexanone
Concen: 3.81 ug/L
RT: 8.149 min Scan# 2211
Delta R.T. 0.009 min
Lab File: VV020656.D
Acq: 17 Mar 2021 15:41

Tgt Ion: 43	Resp: 14525
Ion Ratio	Lower Upper
43 100	
58 46.4	41.8 62.6
57 5.6	15.0 22.4#
100 7.4	8.9 13.3#

Instrument :
MSVOA_V
ClientSampleId :
BG509

Manual Integrations
APPROVED

MMDadoda
3/19/2021 11:28:25 AM

