




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030234.D
 Acq On : 17 Mar 2023 13:06
 Operator : SY/MD
 Sample : 01947-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB931

Manual IntegrationsAPPROVED

Quant Time: Mar 17 22:58:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

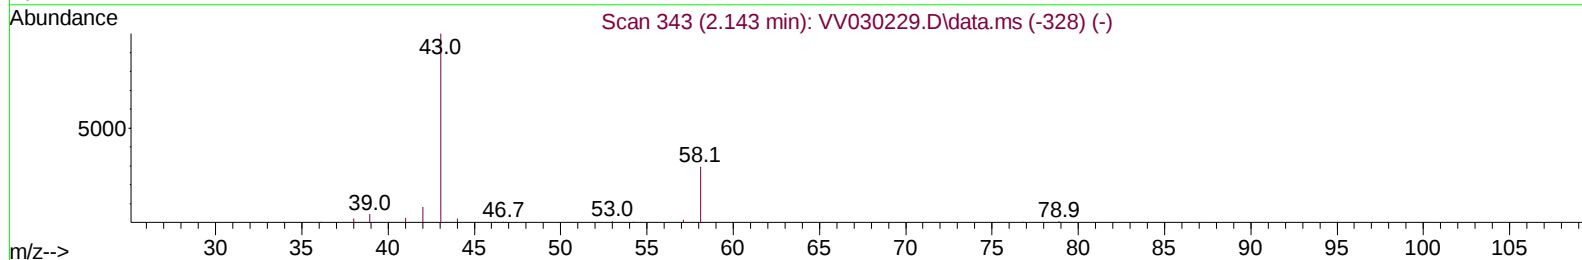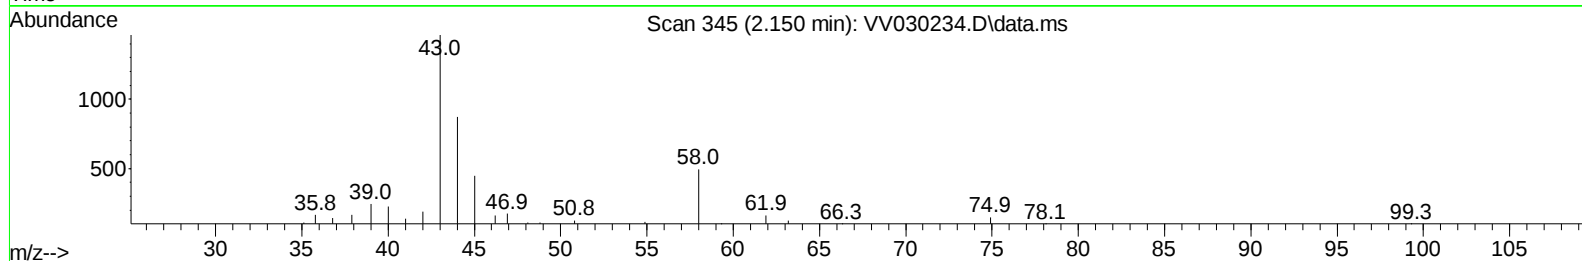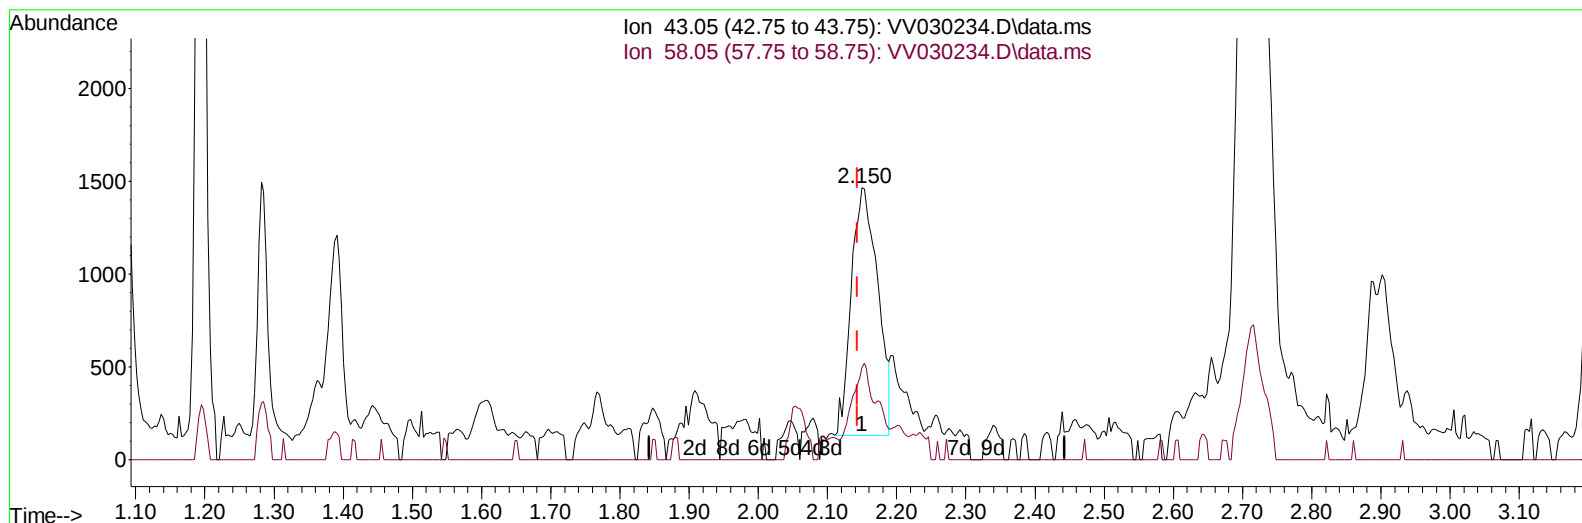

TIC: VV030234.D\data.ms

(13) Acetone (T)

2.150min (+ 0.007) 3.11 ug/L

response 3542

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	20.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030234.D
 Acq On : 17 Mar 2023 13:06
 Operator : SY/MD
 Sample : 01947-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB931

Manual IntegrationsAPPROVED

Quant Time: Mar 17 22:58:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

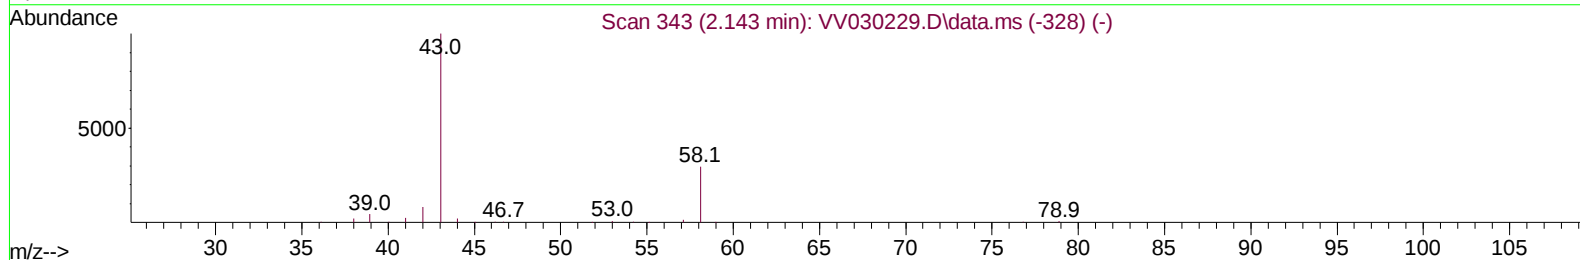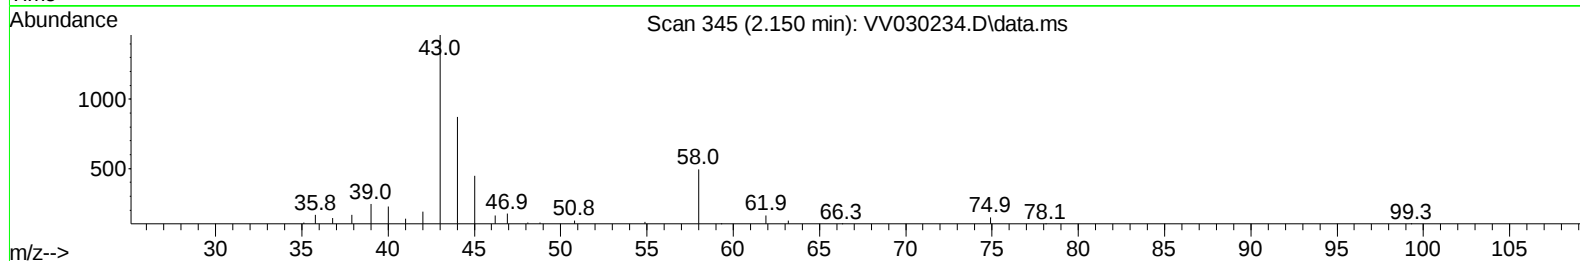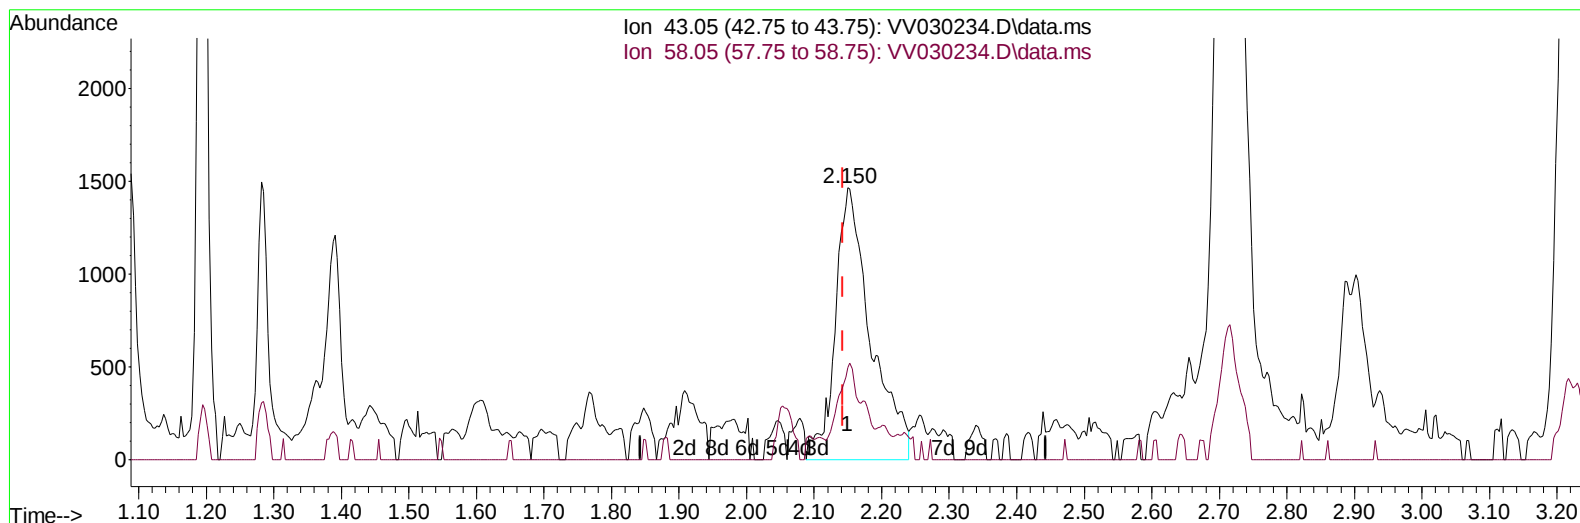

TIC: VV030234.D\data.ms

(13) Acetone (T)

2.150min (+ 0.007) 4.71 ug/L m

response 5357

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	14.70	13.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030234.D
 Acq On : 17 Mar 2023 13:06
 Operator : SY/MD
 Sample : 01947-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB931

Manual IntegrationsAPPROVED

Quant Time: Mar 17 22:58:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		129030	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117		124979	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		64639	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.282	65		32500	3.893	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%	
7) Chloroethane-d5	1.539	69		31129	3.972	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.400%	
11) 1,1-Dichloroethene-d2	2.066	63		53133	3.096	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.822	46		79946	51.937	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.880%	
24) Chloroform-d	4.262	84		72080	4.226	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%	
26) 1,2-Dichloroethane-d4	4.957	65		36557	5.251	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%	
32) Benzene-d6	4.973	84		131611	3.914	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.200%	
36) 1,2-Dichloropropane-d6	5.998	67		42594	4.210	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.200%	
41) Toluene-d8	7.252	98		116595	3.658	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.200%	
43) trans-1,3-Dichloroprop...	7.561	79		14513	4.193	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.800%	
46) 2-Hexanone-d5	8.037	63		63132	44.087	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.180%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		31645	4.397	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.000%	
66) 1,2-Dichlorobenzene-d4	11.571	152		50362	4.605	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.000%	
Target Compounds							
						Qvalue	
13) Acetone	2.150	43		5357m	4.709	ug/L	
17) Methyl tert-butyl Ether	2.712	73		74864	4.421	ug/L #	91
35) Methylcyclohexane	6.066	83		2037	0.141	ug/L #	60
42) Toluene	7.330	91		5461	0.148	ug/L	89
51) Chlorobenzene	8.825	112		44059	1.767	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030234.D
Acq On : 17 Mar 2023 13:06
Operator : SY/MD
Sample : 01947-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB931

Manual IntegrationsAPPROVED

Quant Time: Mar 17 22:58:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

