




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030237.D
 Acq On : 17 Mar 2023 15:49
 Operator : SY/MD
 Sample : 01996-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A26

Manual IntegrationsAPPROVED

Quant Time: Mar 17 22:59:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

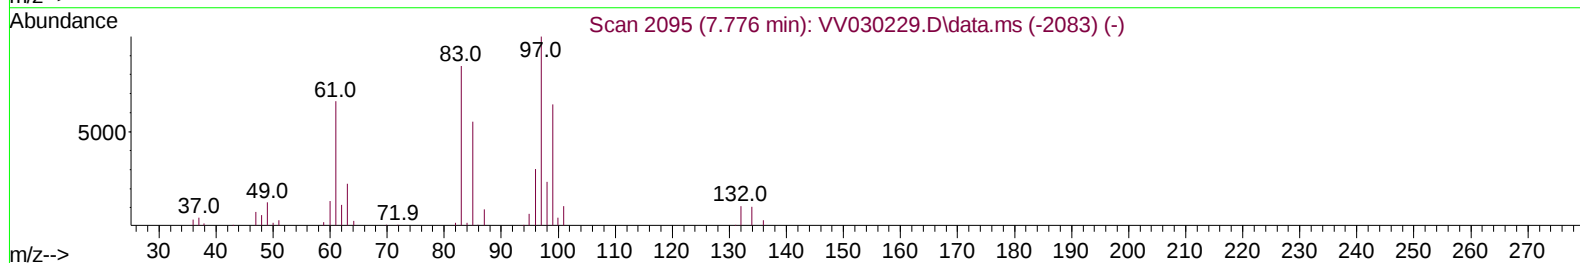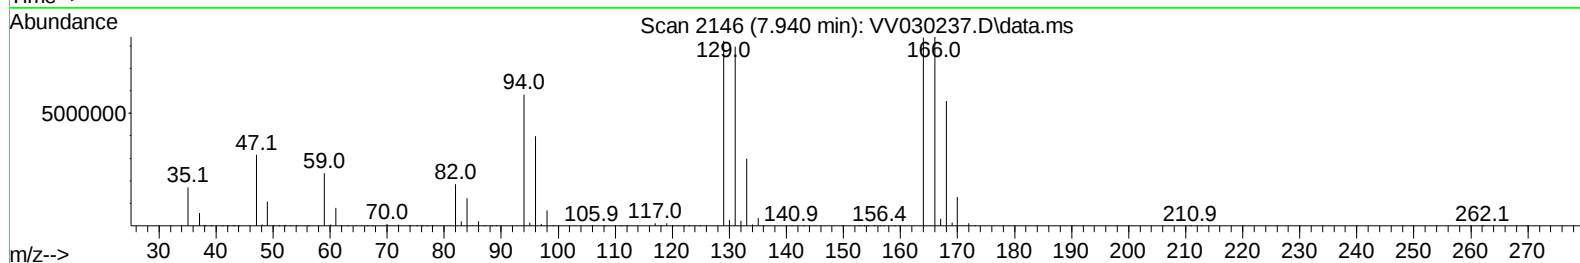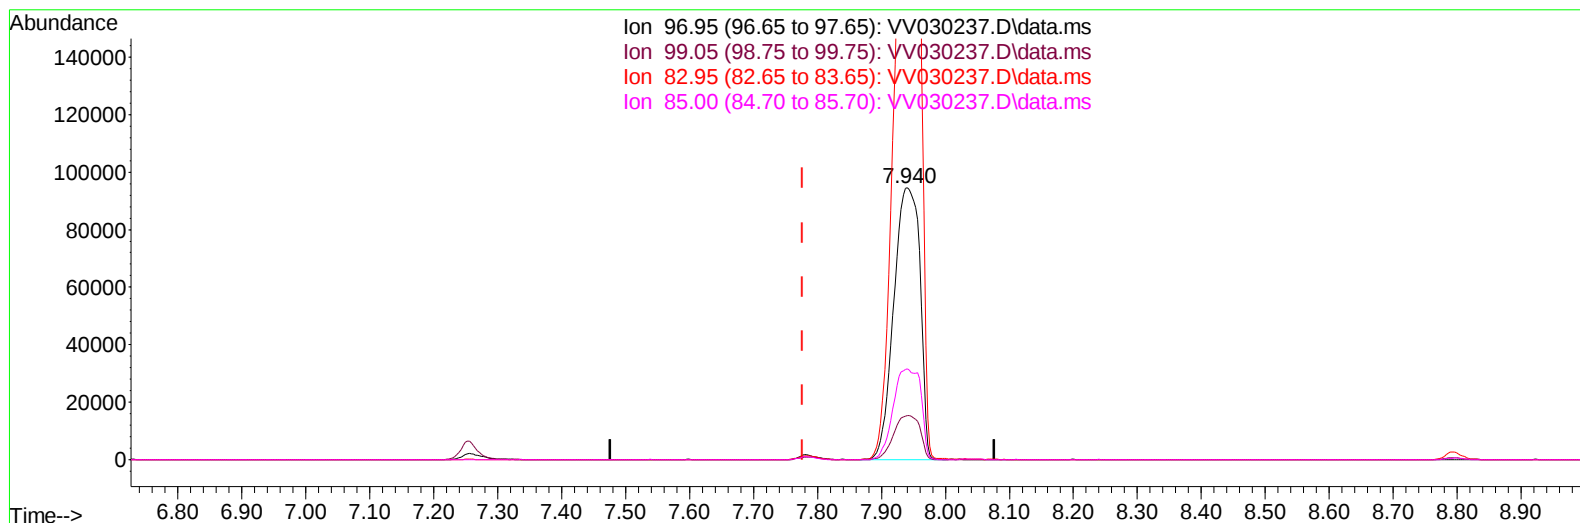

TIC: VV030237.D\data.ms

(45) 1,1,2-Trichloroethane (T)

7.940min (+ 0.164) 45.42 ug/L

response 268125

Ion	Exp%	Act%
96.95	100.00	100.00
99.05	60.90	16.08#
82.95	82.50	199.12#
85.00	55.50	33.34#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030237.D
Acq On : 17 Mar 2023 15:49
Operator : SY/MD
Sample : 01996-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A26

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

Quant Time: Mar 17 22:59:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

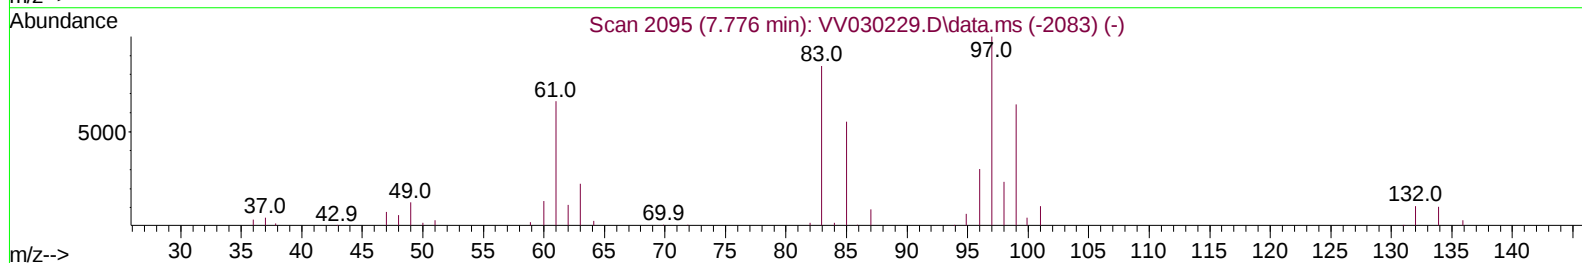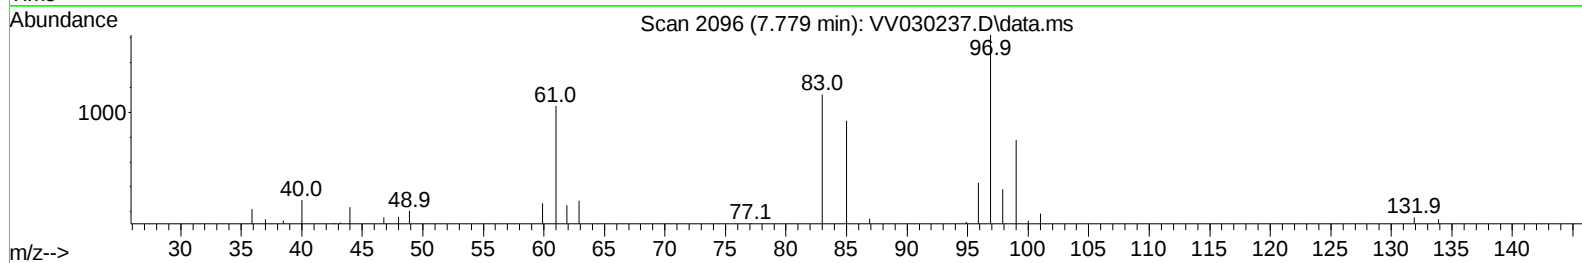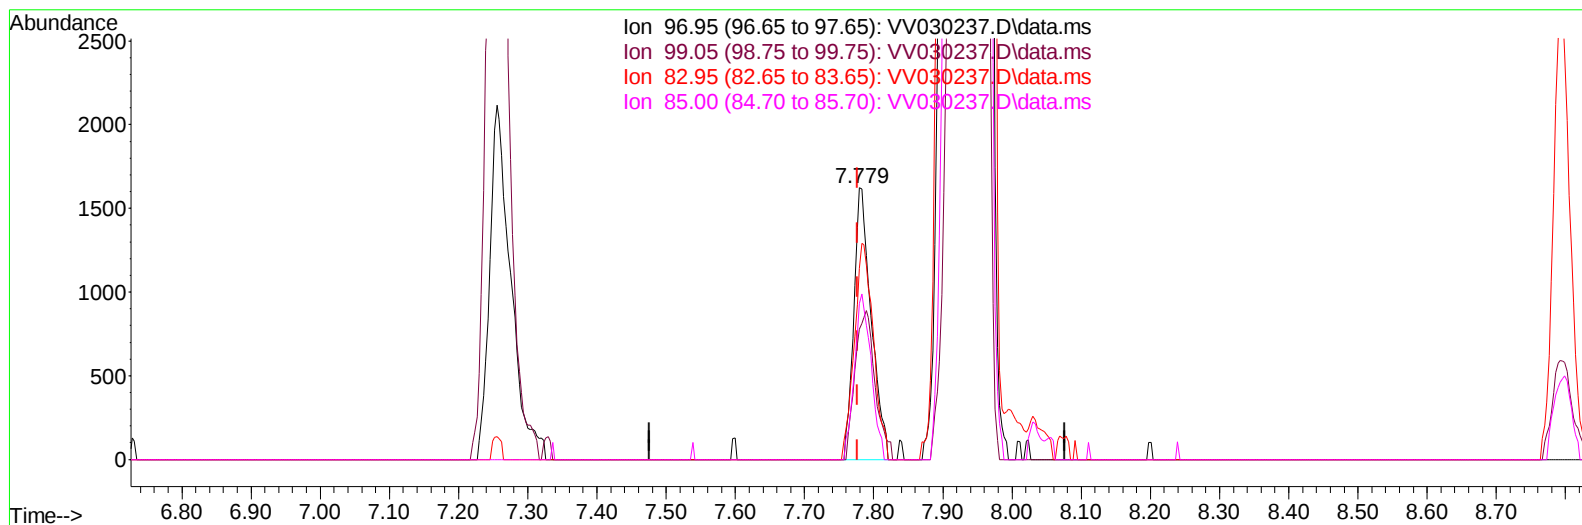

TIC: VV030237.D\data.ms

(45) 1,1,2-Trichloroethane (T)

7.779min (+ 0.003) 0.48 ug/L m

response 2820

Ion	Exp%	Act%
96.95	100.00	100.00
99.05	60.90	47.90
82.95	82.50	70.35
85.00	55.50	57.52

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030237.D
 Acq On : 17 Mar 2023 15:49
 Operator : SY/MD
 Sample : 01996-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0A26

Manual IntegrationsAPPROVED

Quant Time: Mar 17 22:59:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
 Supervised By :Mahesh Dadoda 03/22/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		130266	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.796	117		118735	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		59821	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.281	65		32754	3.886	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%	
7) Chloroethane-d5	1.539	69		30668	3.876	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.600%	
11) 1,1-Dichloroethene-d2	2.076	63		721835	41.655	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	833.200%#	
20) 2-Butanone-d5	3.812	46		80666	51.908	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.820%	
24) Chloroform-d	4.262	84		74580	4.332	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.600%	
26) 1,2-Dichloroethane-d4	4.953	65		36226	5.154	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.000%	
32) Benzene-d6	4.973	84		129090	4.040	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.800%	
36) 1,2-Dichloropropane-d6	5.998	67		41208	4.287	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.800%	
41) Toluene-d8	7.252	98		114956	3.796	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.000%	
43) trans-1,3-Dichloroprop...	7.564	79		14955	4.548	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.000%	
46) 2-Hexanone-d5	8.037	63		66314	48.744	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.480%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		27633	4.041	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.800%	
66) 1,2-Dichlorobenzene-d4	11.570	152		43505	4.298	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.000%	
Target Compounds							
						Qvalue	
12) 1,1-Dichloroethene	2.076	96	1154414	132.051	ug/L	#	71
19) 1,1-Dichloroethane	3.124	63	21305	1.375	ug/L		95
22) cis-1,2-Dichloroethene	3.825	96	36301	3.949	ug/L		91
25) Chloroform	4.288	83	66098	4.101	ug/L		99
29) 1,1,1-Trichloroethane	4.526	97	158035	11.330	ug/L		96
31) Carbon tetrachloride	4.747	117	60332	4.812	ug/L		97
33) Benzene	5.024	78	15611	0.481	ug/L		100
34) Trichloroethene	5.844	95	3979269	437.938	ug/L		94
45) 1,1,2-Trichloroethane	7.779	97	2820m	0.478	ug/L		
47) Tetrachloroethene	7.943	164	24659453	3161.685	ug/L		85
64) 1,3-Dichlorobenzene	11.127	146	6984	0.390	ug/L		94
65) 1,4-Dichlorobenzene	11.220	146	6026	0.333	ug/L		97
67) 1,2-Dichlorobenzene	11.590	146	8367	0.529	ug/L		98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030237.D
Acq On : 17 Mar 2023 15:49
Operator : SY/MD
Sample : 01996-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0A26

Manual IntegrationsAPPROVED

Quant Time: Mar 17 22:59:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/22/2023
Supervised By :Mahesh Dadoda 03/22/2023

