

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030230.D
 Acq On : 17 Mar 2023 11:32
 Operator : SY/MD
 Sample : VV0317WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK314

Quant Time: Mar 17 22:57:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	121941	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	117074	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	56998	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	35085	4.447	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.000%
7) Chloroethane-d5	1.536	69	32098	4.334	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.600%
11) 1,1-Dichloroethene-d2	2.063	63	55395	3.415	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.200%
20) 2-Butanone-d5	3.838	46	79294	54.508	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.020%
24) Chloroform-d	4.262	84	72000	4.467	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
26) 1,2-Dichloroethane-d4	4.953	65	36967	5.618	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.400%
32) Benzene-d6	4.973	84	132372	4.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	5.998	67	40206	4.242	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.800%
41) Toluene-d8	7.252	98	113258	3.793	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.800%
43) trans-1,3-Dichloroprop...	7.564	79	14829	4.573	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.037	63	61312	45.707	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.420%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	30067	4.459	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	11.571	152	44052	4.568	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.400%
Target Compounds						Qvalue
16) Methylene chloride	2.455	84	2782	0.278	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030230.D
Acq On : 17 Mar 2023 11:32
Operator : SY/MD
Sample : VV0317WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK314

Quant Time: Mar 17 22:57:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

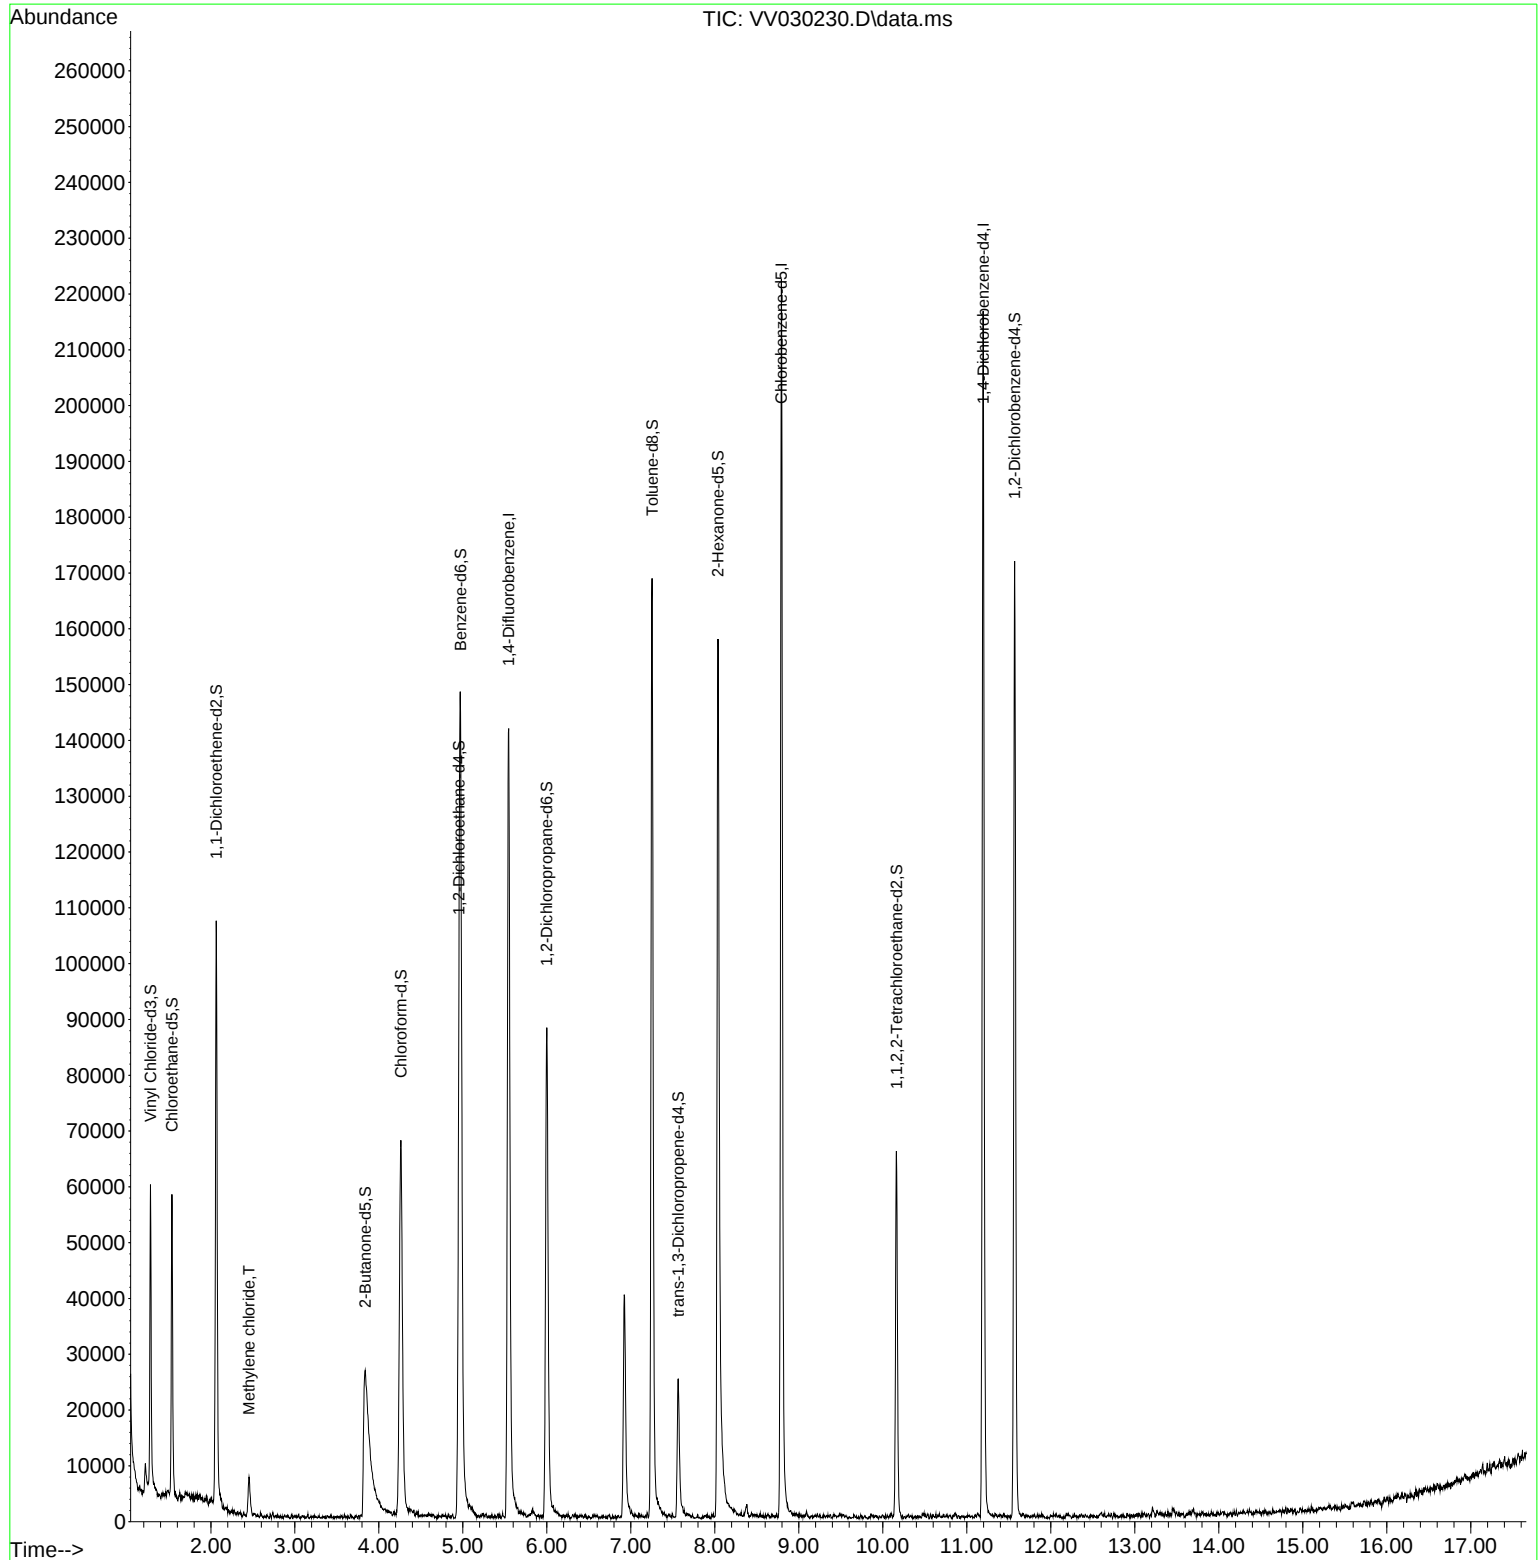

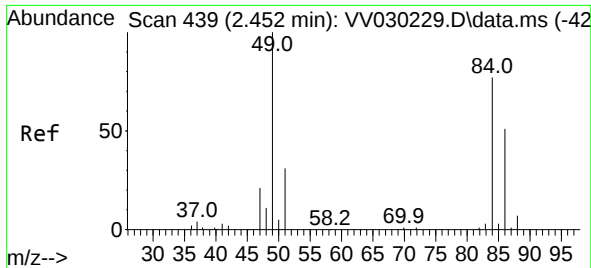

#16
Methylene chloride
Concen: 0.278 ug/L
RT: 2.455 min Scan# 44
Delta R.T. 0.003 min
Lab File: VV030230.D
Acq: 17 Mar 2023 11:32

Instrument :
MSVOA_V
ClientSampleId :
VBLK314

Tgt Ion:	84	Resp:	2782
Ion	Ratio	Lower	Upper
84	100		
86	66.5	44.7	83.1
49	124.3	78.8	146.3

