

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030233.D
 Acq On : 17 Mar 2023 12:41
 Operator : SY/MD
 Sample : 01947-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB941

Quant Time: Mar 17 22:58:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 17 22:49:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.545	114	124509	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	120818	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	58738	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	36451	4.524	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.400%	
7) Chloroethane-d5	1.539	69	33270	4.399	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	88.000%	
11) 1,1-Dichloroethene-d2	2.066	63	57350	3.463	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.200%	
20) 2-Butanone-d5	3.815	46	83380	56.135	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	112.260%	
24) Chloroform-d	4.262	84	76537	4.651	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
26) 1,2-Dichloroethane-d4	4.953	65	39612	5.896	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	118.000%	
32) Benzene-d6	4.973	84	138943	4.274	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.400%	
36) 1,2-Dichloropropane-d6	5.998	67	43106	4.407	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.200%	
41) Toluene-d8	7.252	98	122038	3.960	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.200%	
43) trans-1,3-Dichloroprop...	7.564	79	15730	4.701	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.000%	
46) 2-Hexanone-d5	8.037	63	65025	46.972	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.940%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	30239	4.346	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.000%	
66) 1,2-Dichlorobenzene-d4	11.570	152	48858	4.916	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.400%	
Target Compounds						
13) Acetone	2.143	43	4889	4.453	ug/L	Qvalue 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030233.D
Acq On : 17 Mar 2023 12:41
Operator : SY/MD
Sample : 01947-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB941

Quant Time: Mar 17 22:58:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 17 22:49:08 2023
Response via : Initial Calibration

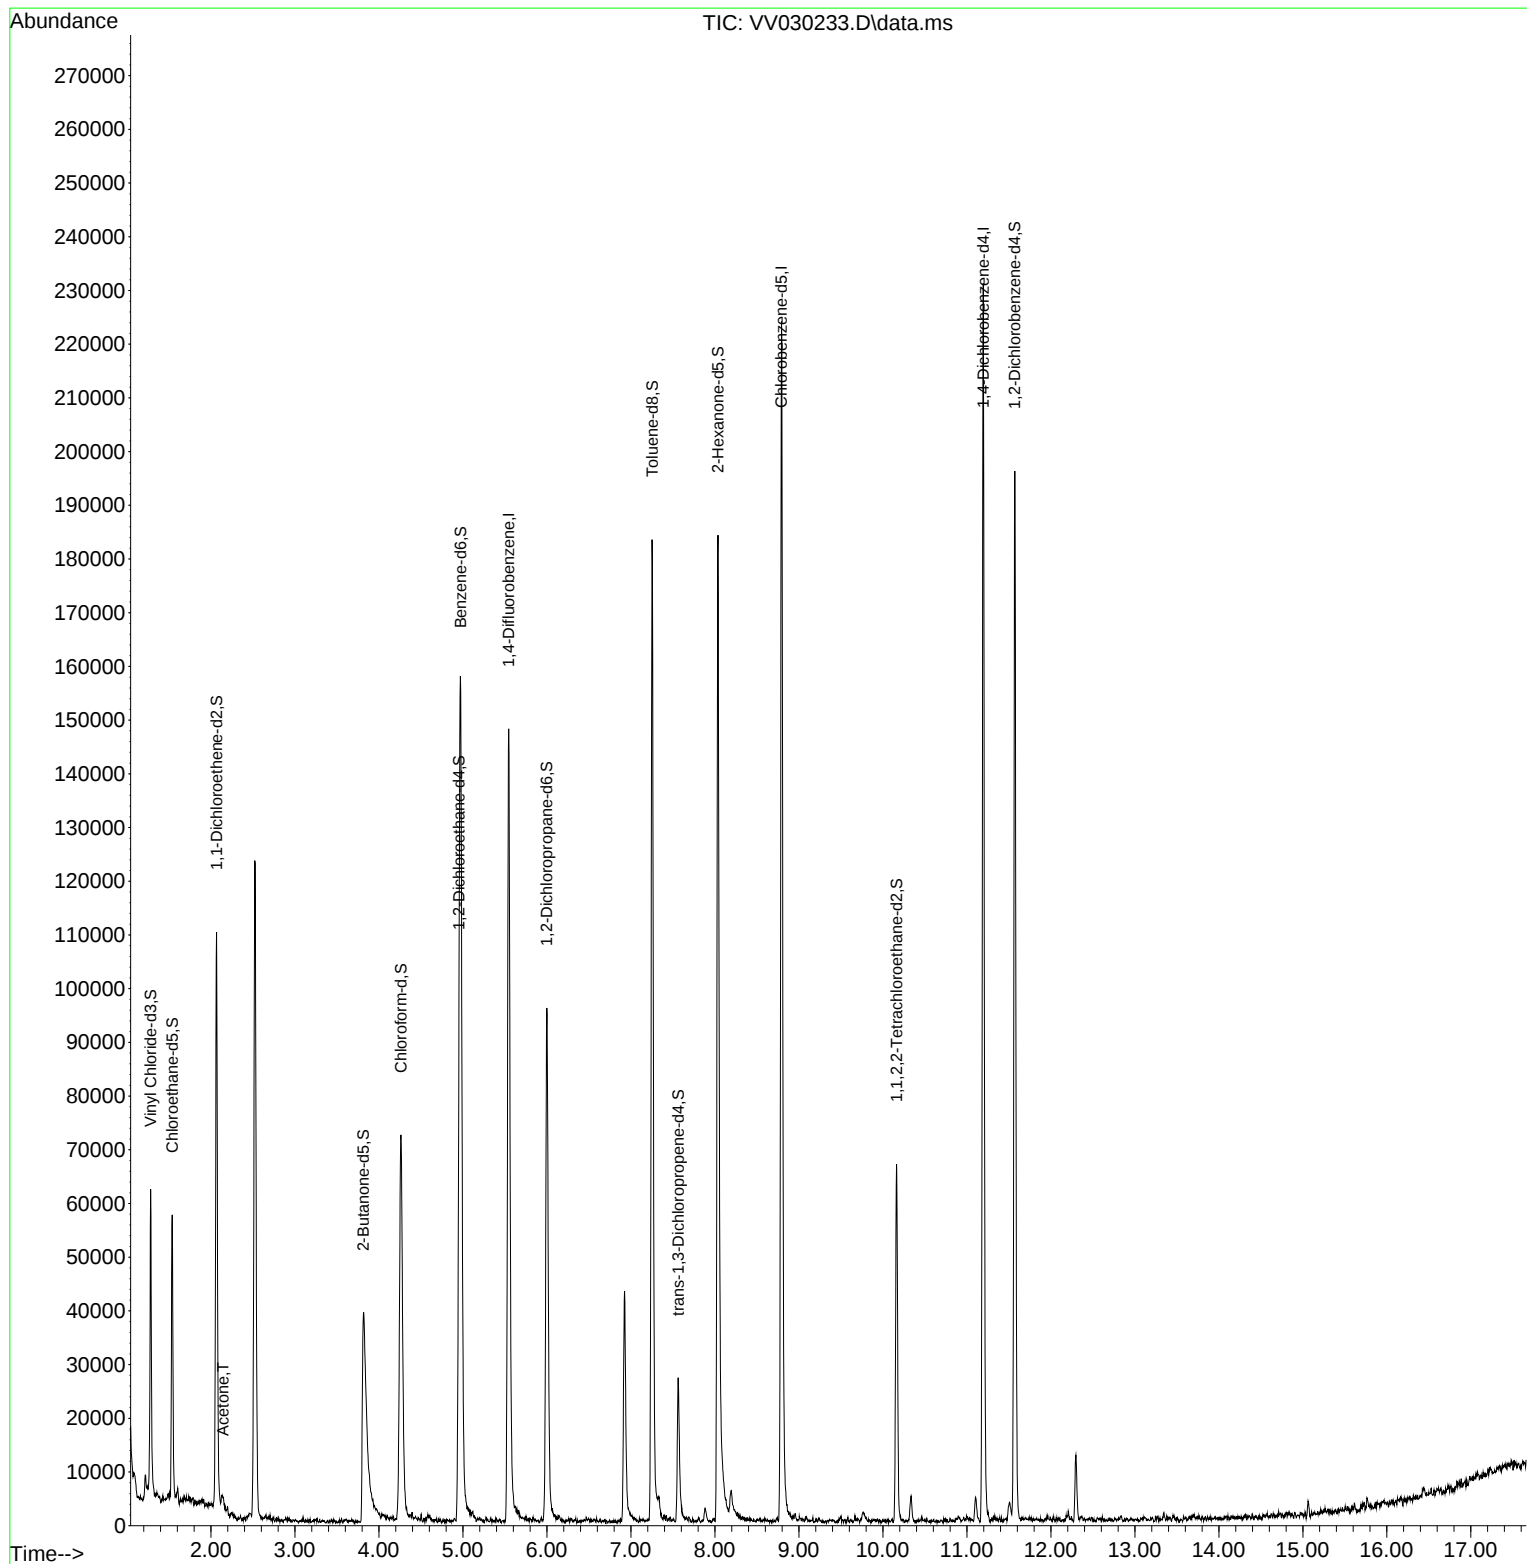

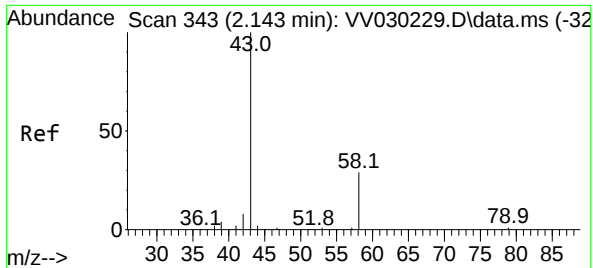

#13
 Acetone
 Concen: 4.453 ug/L
 RT: 2.143 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV030233.D
 Acq: 17 Mar 2023 12:41

Instrument :
 MSVOA_V
 ClientSampleId :
 CB941

Tgt Ion: 43 Resp: 4889
 Ion Ratio Lower Upper
 43 100
 58 26.2 0.0 29.4

