

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
 Data File : VV030244.D
 Acq On : 17 Mar 2023 19:34
 Operator : SY/MD
 Sample : VIBLK281
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK281

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	67	rBV	29025	41986	12.09%	1.241%
2	1.281	69	75	92	rVB	48889	61056	17.58%	1.805%
3	1.539	148	155	169	rVB	46981	56891	16.38%	1.682%
4	2.066	308	319	337	rVB	96355	144934	41.72%	4.285%
5	2.455	428	440	460	rBV	107157	182884	52.64%	5.407%
6	3.825	852	866	895	rBV3	33688	136093	39.17%	4.024%
7	4.262	984	1002	1027	rBV2	62535	165478	47.63%	4.893%
8	4.969	1204	1222	1245	rBV2	134128	347398	100.00%	10.272%
9	5.545	1388	1401	1424	rBV	130382	274065	78.89%	8.104%
10	5.844	1485	1494	1508	rBV	5635	11169	3.22%	0.330%
11	5.998	1528	1542	1560	rBV	81290	177848	51.19%	5.259%
12	6.921	1817	1829	1845	rBV	35259	68955	19.85%	2.039%
13	7.252	1921	1932	1953	rBV	150870	272432	78.42%	8.055%
14	7.564	2018	2029	2041	rBV2	22181	39386	11.34%	1.165%
15	7.915	2126	2138	2158	rVB2	48147	84855	24.43%	2.509%
16	8.037	2166	2176	2213	rBV	157151	316635	91.14%	9.362%
17	8.374	2271	2281	2292	rBV3	7164	12672	3.65%	0.375%
18	8.792	2399	2411	2438	rBV	199874	337738	97.22%	9.986%
19	10.162	2827	2837	2851	rBV	64904	100357	28.89%	2.967%
20	11.194	3147	3158	3173	rBV	193644	301468	86.78%	8.914%
21	11.570	3262	3275	3293	rBV	152824	247748	71.32%	7.325%




Sum of corrected areas: 3382048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030244.D
Acq On : 17 Mar 2023 19:34
Operator : SY/MD
Sample : VIBLK281
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

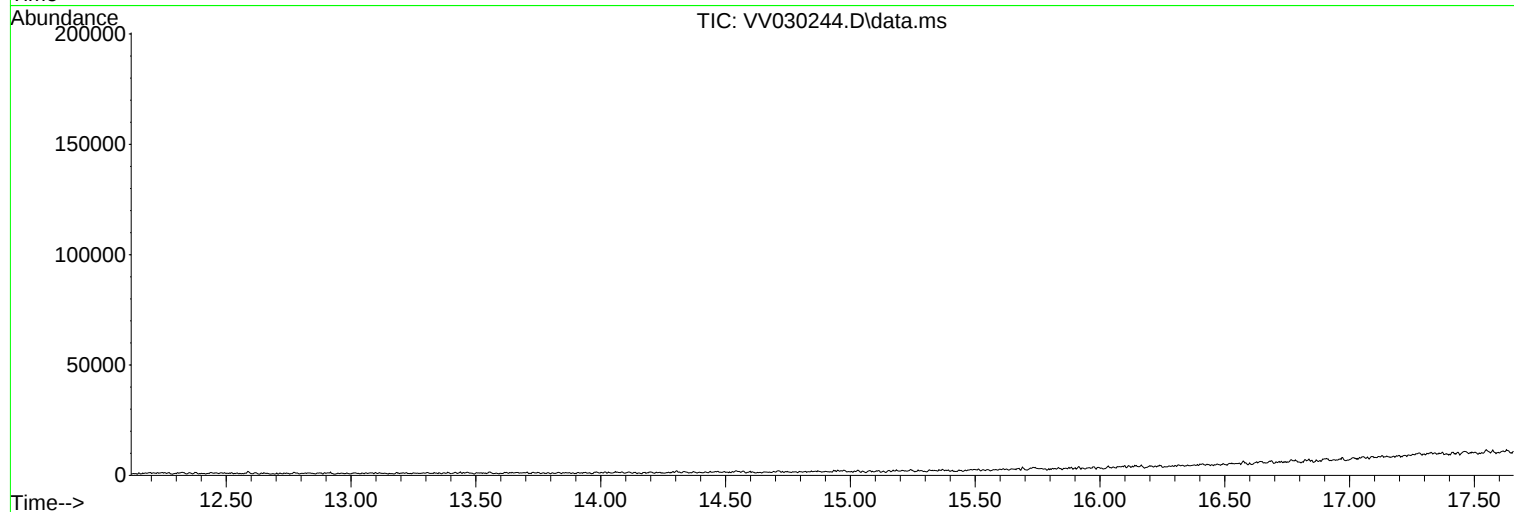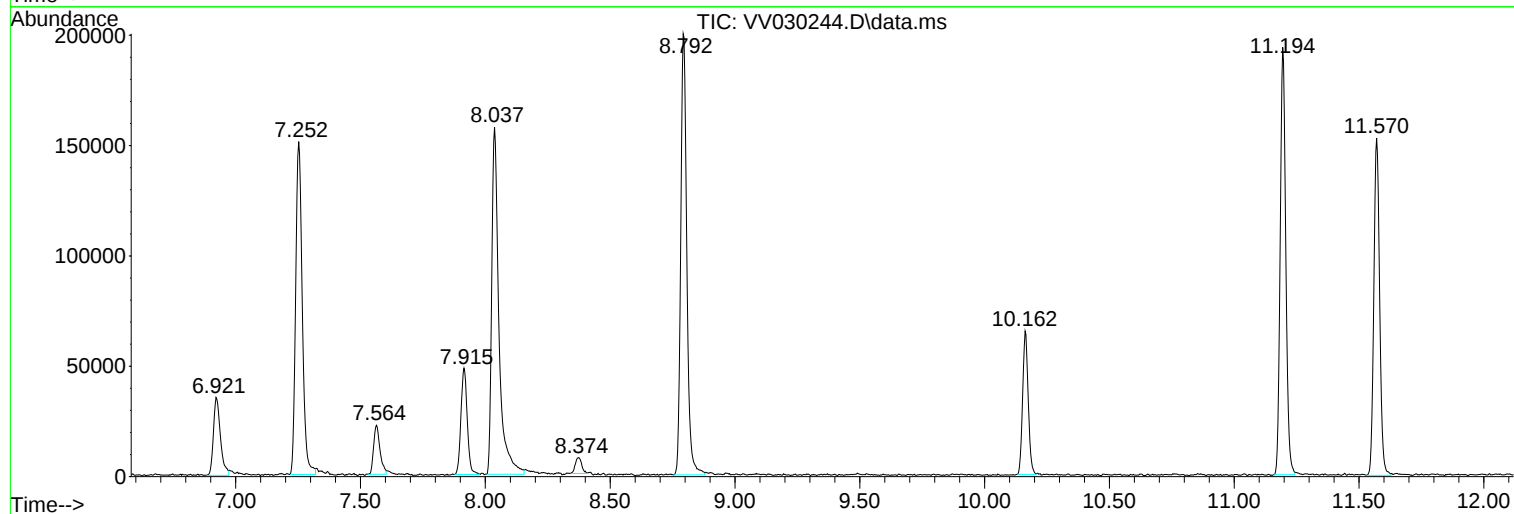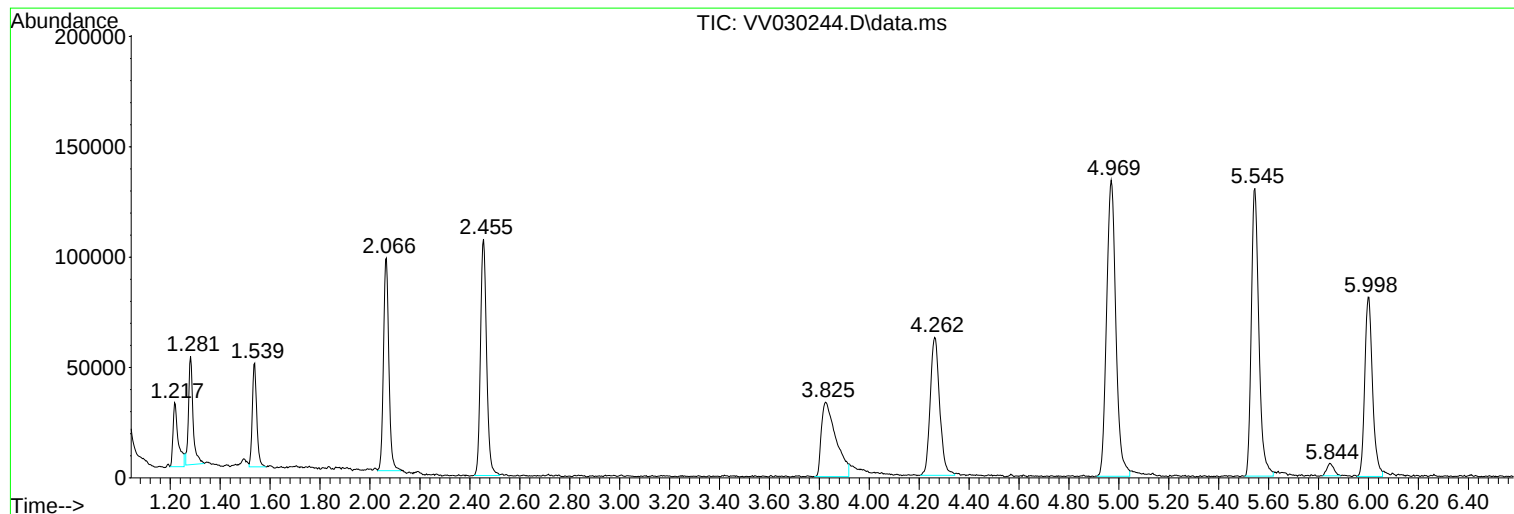

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030244.D
Acq On : 17 Mar 2023 19:34
Operator : SY/MD
Sample : VIBLK281
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030244.D
Acq On : 17 Mar 2023 19:34
Operator : SY/MD
Sample : VIBLK281
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------