
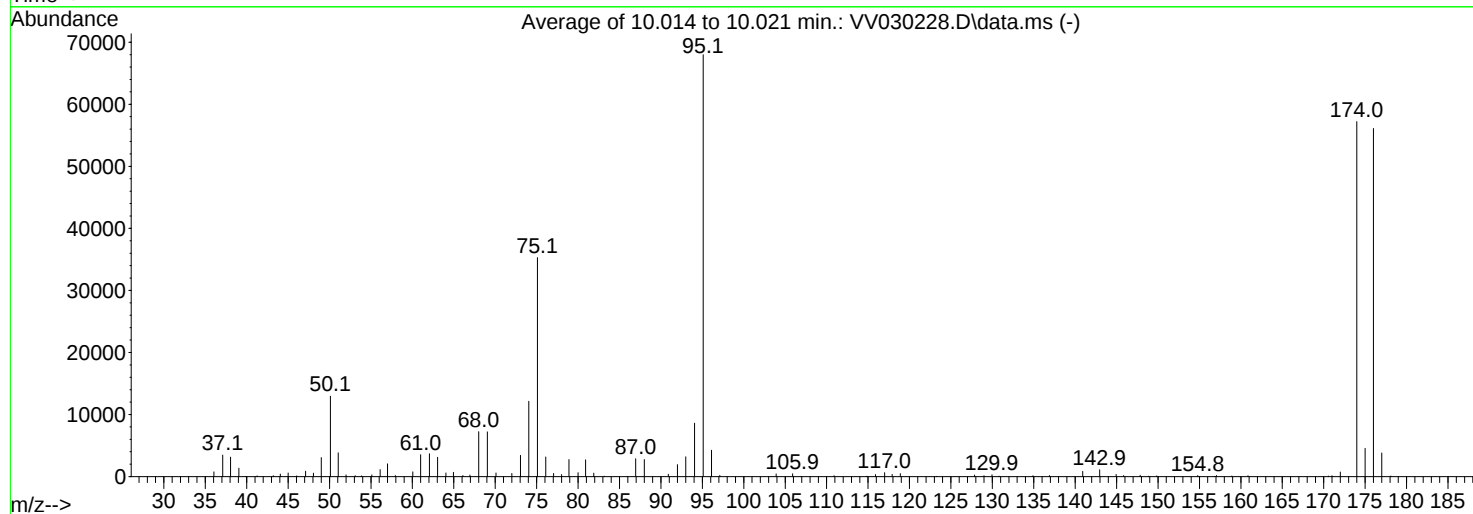


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031723\
Data File : VV030228.D
Acq On : 17 Mar 2023 09:35
Operator : SY/MD
Sample : BFB234
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB234

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 17 22:49:08 2023

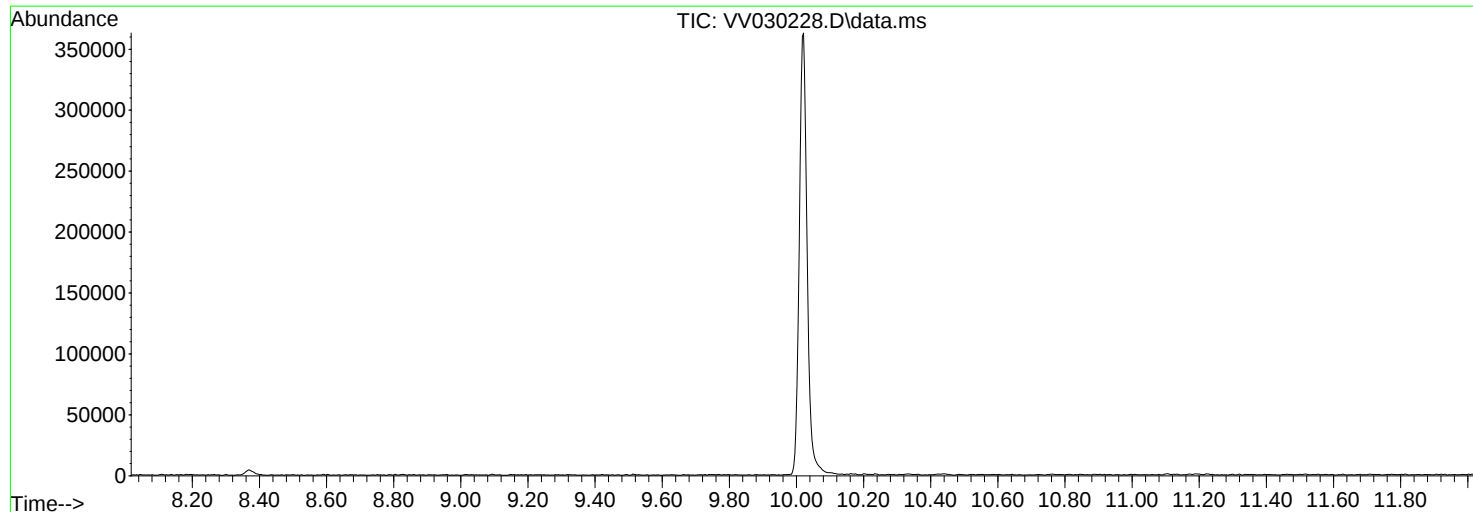

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	12959	PASS
75	95	30	80	51.9	35299	PASS
95	95	100	100	100.0	67981	PASS
96	95	5	9	6.2	4247	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.1	57200	PASS
175	174	5	9	8.0	4556	PASS
176	174	95	105	98.1	56107	PASS
177	176	5	10	6.8	3798	PASS

m/z	Abundance
36.80	102.0
39.30	110.0
39.90	279.0
42.20	145.0
42.80	111.0
44.00	283.0
45.30	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
36.10	709.0
37.10	3250.0
38.00	3164.0
39.10	1340.0
39.80	284.0
41.20	110.0
43.20	166.0
44.10	623.0
45.00	579.0
46.00	150.0
47.10	825.0
48.00	471.0
49.00	3038.0
50.10	12293.0
51.10	3611.0
52.00	247.0
53.10	136.0
53.90	123.0
55.10	246.0
56.10	1040.0
57.00	1970.0
58.00	132.0
60.10	835.0
61.00	3204.0
62.00	3405.0
63.10	2987.0
64.10	486.0
65.00	575.0
66.10	165.0
67.00	226.0
68.00	6726.0
69.00	6799.0
70.10	547.0
72.00	466.0
73.10	3078.0
74.00	11307.0
75.10	32648.0
76.10	2967.0
77.00	358.0
78.00	340.0
78.90	2621.0
80.00	590.0
80.90	2471.0
81.90	509.0
86.90	2528.0
88.00	2592.0
90.90	364.0
92.00	2002.0
93.00	2974.0
94.10	7915.0
95.10	63152.0
96.10	3937.0
97.10	159.0
103.90	366.0
105.90	482.0
106.90	106.0
110.90	156.0
114.80	105.0
115.90	307.0
117.00	607.0
117.90	317.0
118.90	488.0
127.80	270.0
129.00	136.0
130.00	277.0
130.80	126.0
134.90	124.0
137.00	133.0
140.90	763.0
142.90	989.0
145.00	351.0
145.90	162.0
147.90	234.0
148.90	116.0
149.80	119.0
154.80	187.0
156.80	113.0
157.00	116.0
160.80	110.0
170.60	125.0
171.10	127.0
172.00	674.0
174.00	51544.0
175.00	4030.0
176.00	50408.0
177.00	3533.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
36.00	766.0
37.10	3563.0
38.00	3204.0
39.00	1368.0
39.80	289.0
41.30	110.0
43.20	147.0
44.10	731.0
45.00	616.0
46.10	119.0
47.10	891.0
48.00	550.0
49.00	3176.0
50.10	13424.0
51.10	3982.0
52.00	284.0
53.10	167.0
53.90	115.0
55.10	270.0
56.10	1169.0
57.00	2121.0
58.00	163.0
60.10	784.0
61.00	3581.0
62.00	3784.0
63.00	3175.0
64.00	589.0
64.90	700.0
66.10	165.0
66.90	244.0
68.00	7537.0
69.10	7461.0
70.10	588.0
72.00	531.0
73.00	3552.0
74.00	12487.0
75.10	36768.0
76.10	3263.0
77.10	497.0
78.00	319.0
78.90	2848.0
80.00	653.0
80.90	2793.0
81.90	571.0
83.20	111.0
87.00	2968.0
88.00	2846.0
90.90	349.0
92.00	1985.0
93.00	3273.0
94.10	8912.0
95.10	70680.0
96.10	4387.0
97.10	210.0
103.90	450.0
105.90	450.0
110.90	166.0
114.90	111.0
115.90	326.0
117.00	663.0
117.90	383.0
118.90	491.0
123.30	104.0
127.80	267.0
129.00	159.0
129.90	309.0
130.80	108.0
134.90	141.0
136.90	148.0
140.90	862.0
142.90	1128.0
145.00	364.0
145.90	159.0
147.90	229.0
148.80	120.0
149.90	118.0
154.80	179.0
157.10	171.0
158.90	112.0
160.90	144.0
170.50	131.0
171.00	142.0
172.00	755.0
174.00	59024.0
175.00	4752.0
176.00	57904.0
177.00	3955.0
178.10	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
36.00	803.0
37.10	3605.0
38.10	3068.0
39.00	1356.0
39.90	284.0
41.20	107.0
42.80	106.0
43.20	123.0
44.10	728.0
45.00	557.0
46.10	123.0
47.10	857.0
48.10	614.0
49.00	2985.0
50.10	13161.0
51.00	3931.0
52.00	298.0
53.10	157.0
53.80	109.0
55.10	265.0
56.10	1179.0
57.00	2029.0
57.90	184.0
60.00	685.0
61.00	3739.0
62.10	3814.0
63.00	3138.0
64.00	645.0
64.90	775.0
66.10	150.0
66.90	264.0
68.00	7440.0
69.10	7387.0
70.10	625.0
72.00	557.0
73.00	3656.0
74.10	12589.0
75.10	36480.0
76.10	3223.0
77.10	639.0
78.00	326.0
78.90	2793.0
80.00	694.0
80.90	2859.0
81.90	556.0
83.10	121.0
85.90	121.0
87.00	3103.0
88.00	2814.0
90.90	378.0
92.00	1806.0
93.00	3333.0
94.00	8998.0
95.10	70112.0
96.10	4418.0
97.10	204.0
103.90	442.0
105.90	398.0
110.90	139.0
115.90	312.0
117.00	661.0
117.90	386.0
118.90	446.0
127.90	234.0
129.00	170.0
129.90	327.0
134.90	143.0
136.80	186.0
140.90	908.0
143.00	1183.0
144.90	329.0
145.80	147.0
147.80	212.0
149.90	107.0
154.80	167.0
157.00	199.0
158.90	129.0
160.90	141.0
170.90	181.0
172.00	787.0
174.00	61032.0
175.00	4886.0
176.00	60008.0
177.00	3905.0
178.10	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234