
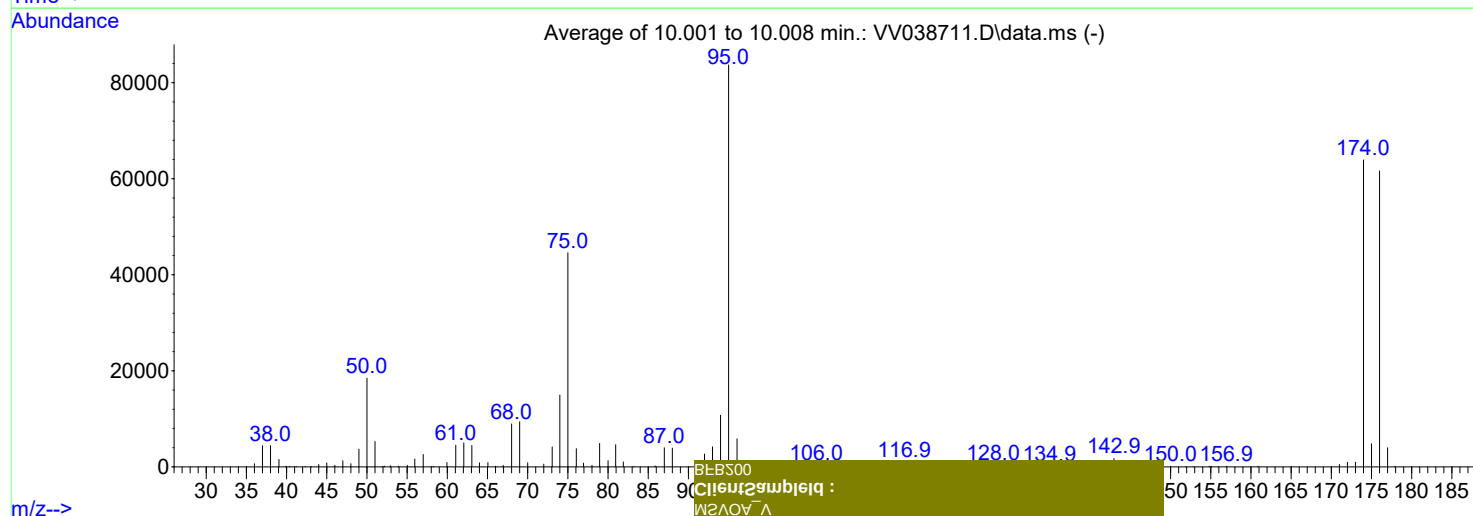


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV031725\
 Data File : VV038711.D
 Acq On : 17 Mar 2025 11:32
 Operator : SY/MD
 Sample : BFB200
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM031724WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 19 08:10:26 2025

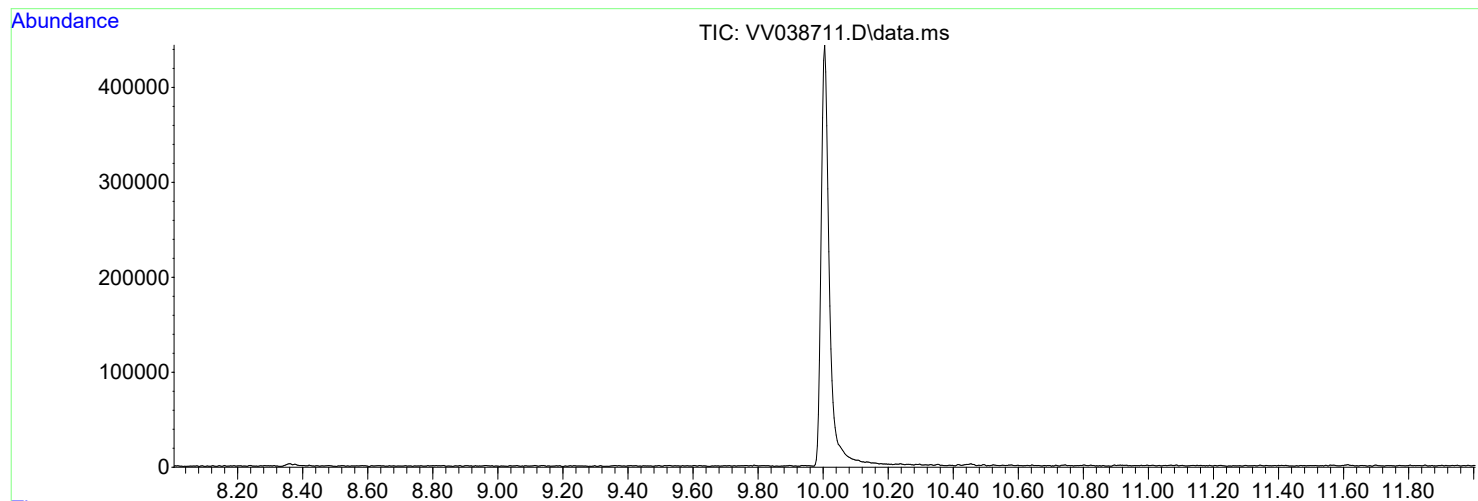

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.1	18493	PASS
75	95	30	80	53.3	44595	PASS
95	95	100	100	100.0	83707	PASS
96	95	5	9	7.0	5844	PASS
173	174	0.00	2	1.5	986	PASS
174	95	50	120	76.4	63912	PASS
175	174	5	9	7.5	4825	PASS
176	174	95	105	96.4	61621	PASS
177	176	5	10	6.5	3985	PASS

m/z	Abundance
36.00	111.0
38.90	154.0
40.00	267.0
44.00	616.0

BFB200
Client Sample :
MS/MS
Instrument :

m/z	Abundance
36.00	841.0
37.00	4529.0
38.00	4327.0
39.10	1802.0
39.90	323.0
40.40	312.0
41.20	101.0
42.30	117.0
43.10	102.0
44.00	1130.0
45.00	934.0
46.00	319.0
47.00	1280.0
48.00	633.0
49.00	3753.0
50.00	18928.0
51.00	5278.0
52.20	251.0
52.90	239.0
53.90	149.0
55.10	251.0
56.00	1575.0
57.00	2496.0
58.30	154.0
60.00	873.0
61.00	4453.0
62.10	4943.0
63.10	4744.0
64.00	791.0
65.00	884.0
66.00	127.0
67.00	337.0
68.00	8850.0
69.00	9462.0
70.00	804.0
72.00	567.0
73.10	4260.0
74.00	15259.0
75.00	45048.0
76.00	4021.0
77.00	777.0
78.00	352.0
78.90	4974.0
80.00	1268.0
81.00	4726.0
81.90	1082.0
83.20	108.0
85.80	163.0
87.00	3922.0
88.00	3831.0
90.90	495.0
92.00	2727.0
93.00	4232.0
94.00	10712.0
95.00	83480.0
96.10	5910.0
97.00	330.0
103.90	421.0
104.80	182.0
105.90	436.0
107.00	164.0
107.90	187.0
111.90	143.0
115.00	124.0
115.90	461.0
116.90	984.0
117.90	336.0
118.80	753.0
127.90	378.0
129.90	372.0
130.90	101.0
135.00	108.0
136.90	169.0
140.90	949.0
141.90	176.0
142.90	1672.0
144.20	169.0
144.90	898.0
145.90	226.0
147.80	143.0
150.00	175.0
151.90	107.0
154.80	174.0
155.90	100.0
156.90	137.0
160.80	135.0
171.00	575.0
172.00	906.0
173.00	1010.0
174.00	62224.0
175.00	4722.0
176.00	60120.0

BFB200
ClientSampleId :
MS200711
Instrument :

177.00

177.90

3944.0

107.0

BEB500

Client Sample :

MSAOA \

Instrument :

m/z	Abundance
36.00	771.0
37.00	4545.0
38.00	4576.0
39.10	1719.0
39.90	375.0
44.00	1137.0
45.00	807.0
46.00	339.0
47.00	1309.0
48.00	717.0
49.00	3754.0
50.00	19168.0
51.00	5477.0
52.10	252.0
52.90	263.0
53.90	158.0
55.00	306.0
55.90	1718.0
57.00	2705.0
58.20	120.0
59.90	937.0
61.00	4632.0
62.10	5206.0
63.10	4557.0
64.00	869.0
65.10	923.0
66.00	157.0
66.90	346.0
68.00	9302.0
69.00	9762.0
70.00	906.0
72.00	611.0
73.10	4271.0
74.00	15512.0
75.00	46112.0
76.10	3864.0
76.90	815.0
78.00	330.0
79.00	5024.0
80.00	1365.0
80.90	4724.0
81.90	1078.0
85.90	217.0
87.00	4088.0
88.00	3983.0
90.90	449.0
92.00	2763.0
93.00	4311.0
94.00	11155.0
95.00	86792.0
96.10	6052.0
97.00	323.0
103.90	453.0
104.80	176.0
106.00	483.0
107.00	166.0
107.90	231.0
110.10	106.0
112.90	140.0
115.00	152.0
115.90	403.0
116.90	1157.0
117.90	353.0
118.80	764.0
127.90	372.0
128.60	125.0
129.90	358.0
134.60	109.0
135.00	122.0
136.90	183.0
140.90	954.0
141.90	164.0
143.00	1796.0
144.10	171.0
144.90	867.0
145.90	223.0
147.80	125.0
150.00	123.0
152.80	103.0
154.80	162.0
155.10	179.0
157.00	158.0
160.80	133.0
171.00	510.0
172.00	1002.0
173.00	996.0
174.00	66168.0
175.00	4985.0
176.00	63960.0
177.00	4070.0
177.90	125.0

BFB200
Client Sample ID :
MS2/MS1
Instrument :

m/z	Abundance
36.00	673.0
37.00	4121.0
38.00	4339.0
39.10	1606.0
39.90	454.0
44.00	1090.0
45.00	732.0
46.00	269.0
47.00	1223.0
48.00	690.0
49.00	3585.0
50.00	17384.0
51.00	5155.0
51.90	266.0
52.90	228.0
53.90	145.0
55.00	338.0
56.00	1620.0
57.00	2544.0
58.00	102.0
59.90	913.0
61.10	4492.0
62.00	4864.0
63.00	4052.0
64.00	877.0
65.10	898.0
66.00	131.0
66.90	303.0
68.00	8689.0
69.00	8959.0
70.00	849.0
72.00	556.0
73.00	3919.0
74.00	14149.0
75.00	42624.0
76.10	3486.0
76.90	789.0
78.00	319.0
78.90	4635.0
80.00	1290.0
80.90	4411.0
81.90	955.0
85.90	258.0
87.00	3947.0
88.00	3877.0
90.90	415.0
92.00	2538.0
93.00	3961.0
94.00	10392.0
95.00	80848.0
96.00	5571.0
97.00	261.0
103.00	117.0
104.00	422.0
104.80	157.0
106.00	467.0
106.90	117.0
107.90	196.0
110.00	117.0
112.30	104.0
113.00	154.0
115.00	180.0
115.80	341.0
116.90	1117.0
117.80	321.0
118.80	771.0
119.60	108.0
128.00	363.0
128.60	122.0
129.90	335.0
134.60	122.0
134.90	130.0
136.90	147.0
140.90	850.0
141.90	151.0
143.00	1774.0
144.90	781.0
145.90	157.0
147.80	113.0
155.10	203.0
157.00	135.0
160.90	123.0
171.00	428.0
172.00	1007.0
173.00	951.0
174.00	63344.0
175.00	4769.0
176.00	60784.0
177.00	3941.0

BFB200
Client Sample ID :
MS2/MS1
Instrument :