

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031819\
 Data File : VV009753.D
 Acq On : 18 Mar 2019 12:57
 Operator : SY/MD
 Sample : K1918-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0971

Quant Time: Mar 19 04:40:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 18 12:32:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	125976	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	118851	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	46136	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45111	53.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.22%
7) Chloroethane-d5	1.56	69	36634	58.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	116.92%
11) 1,1-Dichloroethene-d2	2.12	63	74436	41.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.30%
21) 2-Butanone-d5	3.93	46	56286	111.25	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.25%
24) Chloroform-d	4.40	84	83667	53.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.24%
26) 1,2-Dichloroethane-d4	5.08	65	52294	55.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.44%
32) Benzene-d6	5.10	84	179394	57.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.52%
36) 1,2-Dichloropropane-d6	6.12	67	53237	56.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	112.60%
41) Toluene-d8	7.36	98	168606	56.42	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.84%
43) trans-1,3-Dichloropropene-	7.66	79	24469	54.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	109.44%
47) 2-Hexanone-d5	8.13	63	41219	107.11	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.11%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	74683	52.07	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.14%
64) 1,2-Dichlorobenzene-d4	11.68	152	54008	57.85	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	115.70%


Target Compounds					Ovalue
13) Acetone	2.19	43	3042	6.348 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031819\
Data File : VV009753.D
Acq On : 18 Mar 2019 12:57
Operator : SY/MD
Sample : K1918-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0971

Quant Time: Mar 19 04:40:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 18 12:32:58 2019
Response via : Initial Calibration

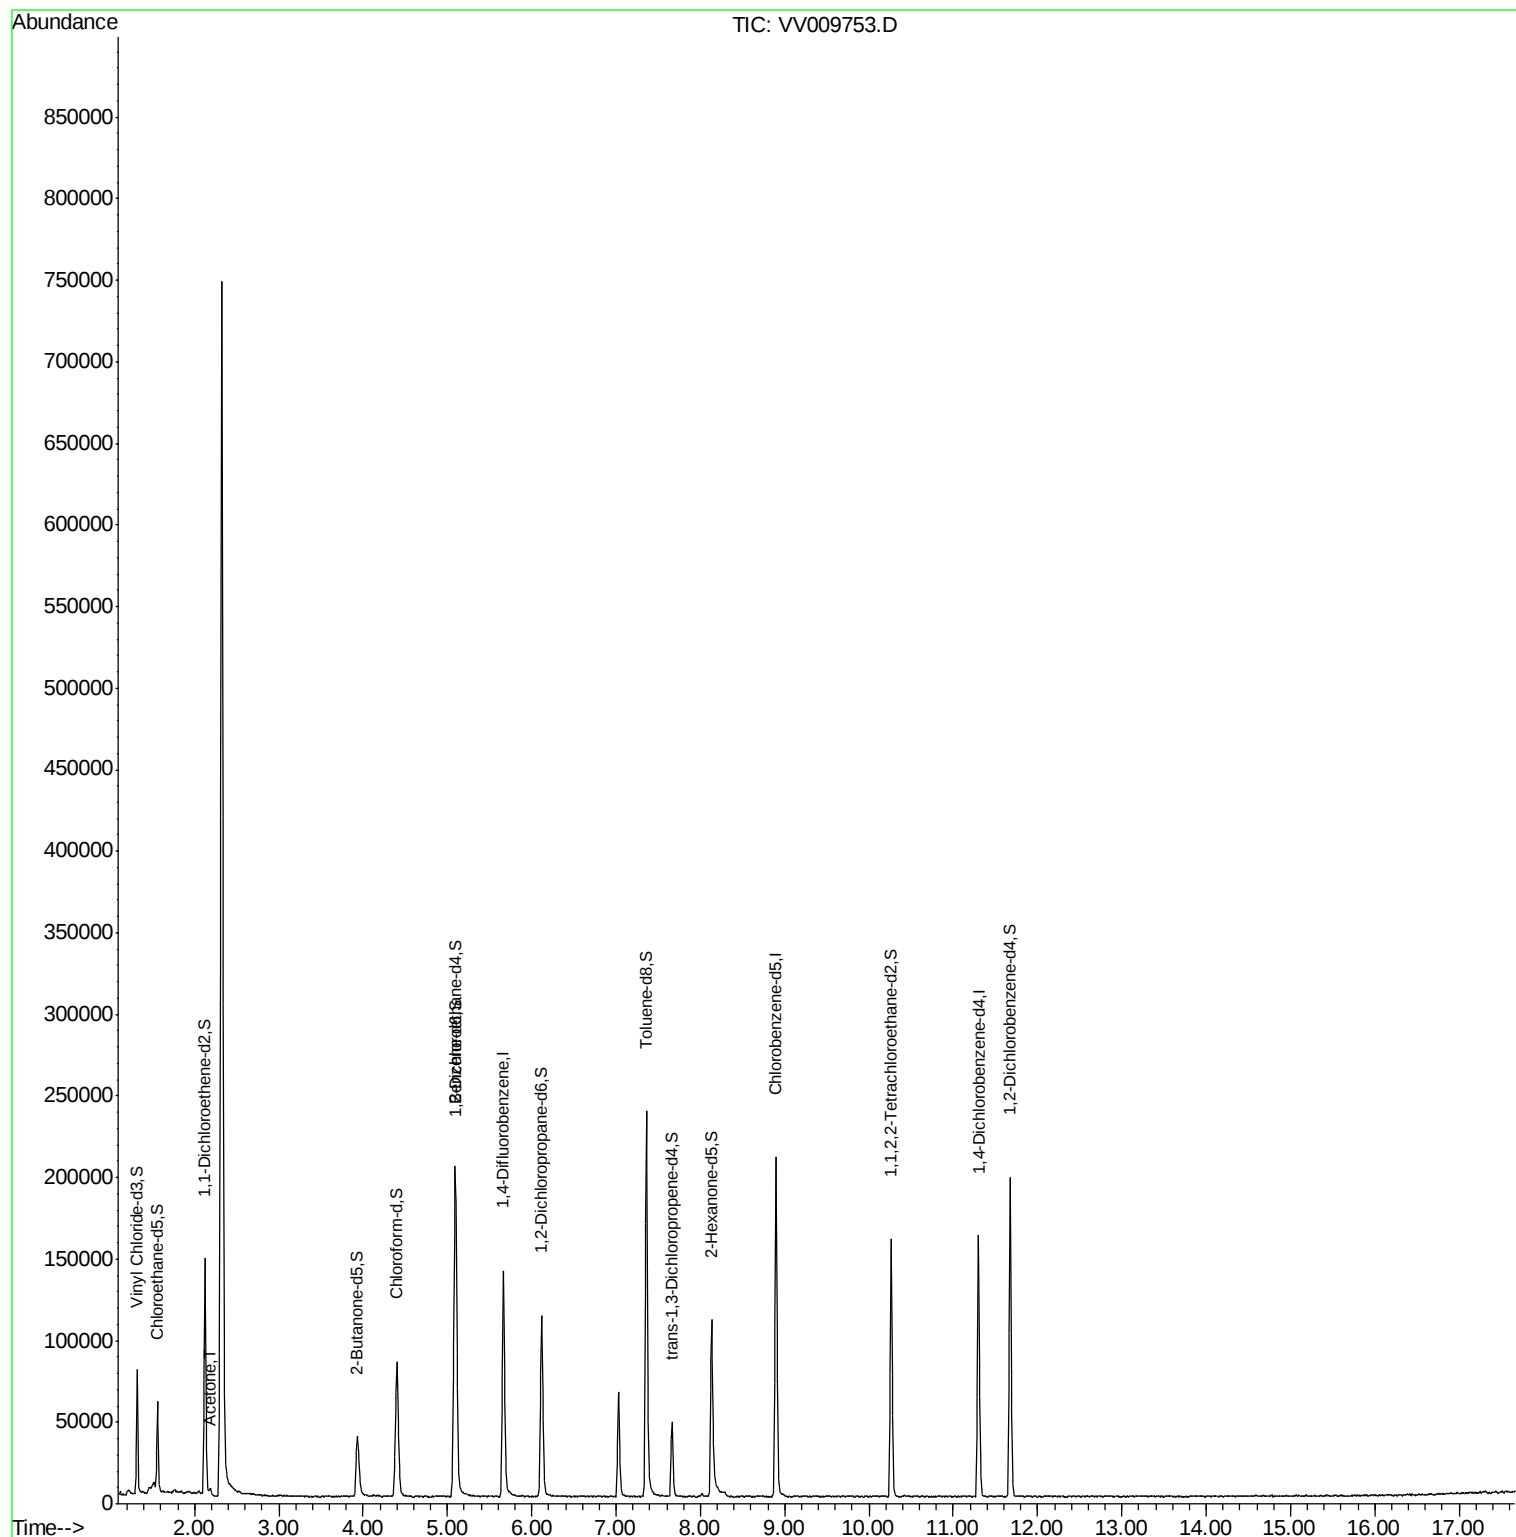

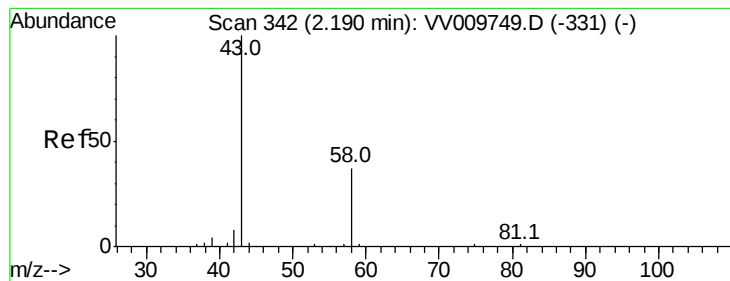

#13

Acetone

Concen: 6.348 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.00 min

Lab File: VV009753.D

Acq: 18 Mar 2019 12:57

Instrument :
MSVOA_V
ClientSampleId :
C0971

Tot Ion: 43 Resp: 3042

Ion Ratio Lower Upper

43 100

58 28.9 0.0 67.8

