

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031819\
 Data File : VV009754.D
 Acq On : 18 Mar 2019 13:21
 Operator : SY/MD
 Sample : K1918-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0991

Quant Time: Mar 19 04:42:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 18 12:32:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	139880	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	133045	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	51525	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45130	47.85	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.70%
7) Chloroethane-d5	1.56	69	37192	53.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.90%
11) 1,1-Dichloroethene-d2	2.12	63	74669	37.18	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.36%
21) 2-Butanone-d5	3.93	46	57136	101.71	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.71%
24) Chloroform-d	4.40	84	82697	47.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.46%
26) 1,2-Dichloroethane-d4	5.08	65	51439	48.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.84%
32) Benzene-d6	5.10	84	178337	51.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.60%
36) 1,2-Dichloropropane-d6	6.12	67	53538	50.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.16%
41) Toluene-d8	7.36	98	167566	50.09	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.18%
43) trans-1,3-Dichloropropene-	7.66	79	24375	48.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.40%
47) 2-Hexanone-d5	8.13	63	42193	97.94	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.94%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	76335	47.54	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.08%
64) 1,2-Dichlorobenzene-d4	11.67	152	54108	51.90	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	3325	6.249 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031819\
 Data File : VV009754.D
 Acq On : 18 Mar 2019 13:21
 Operator : SY/MD
 Sample : K1918-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0991

Quant Time: Mar 19 04:42:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 18 12:32:58 2019
 Response via : Initial Calibration

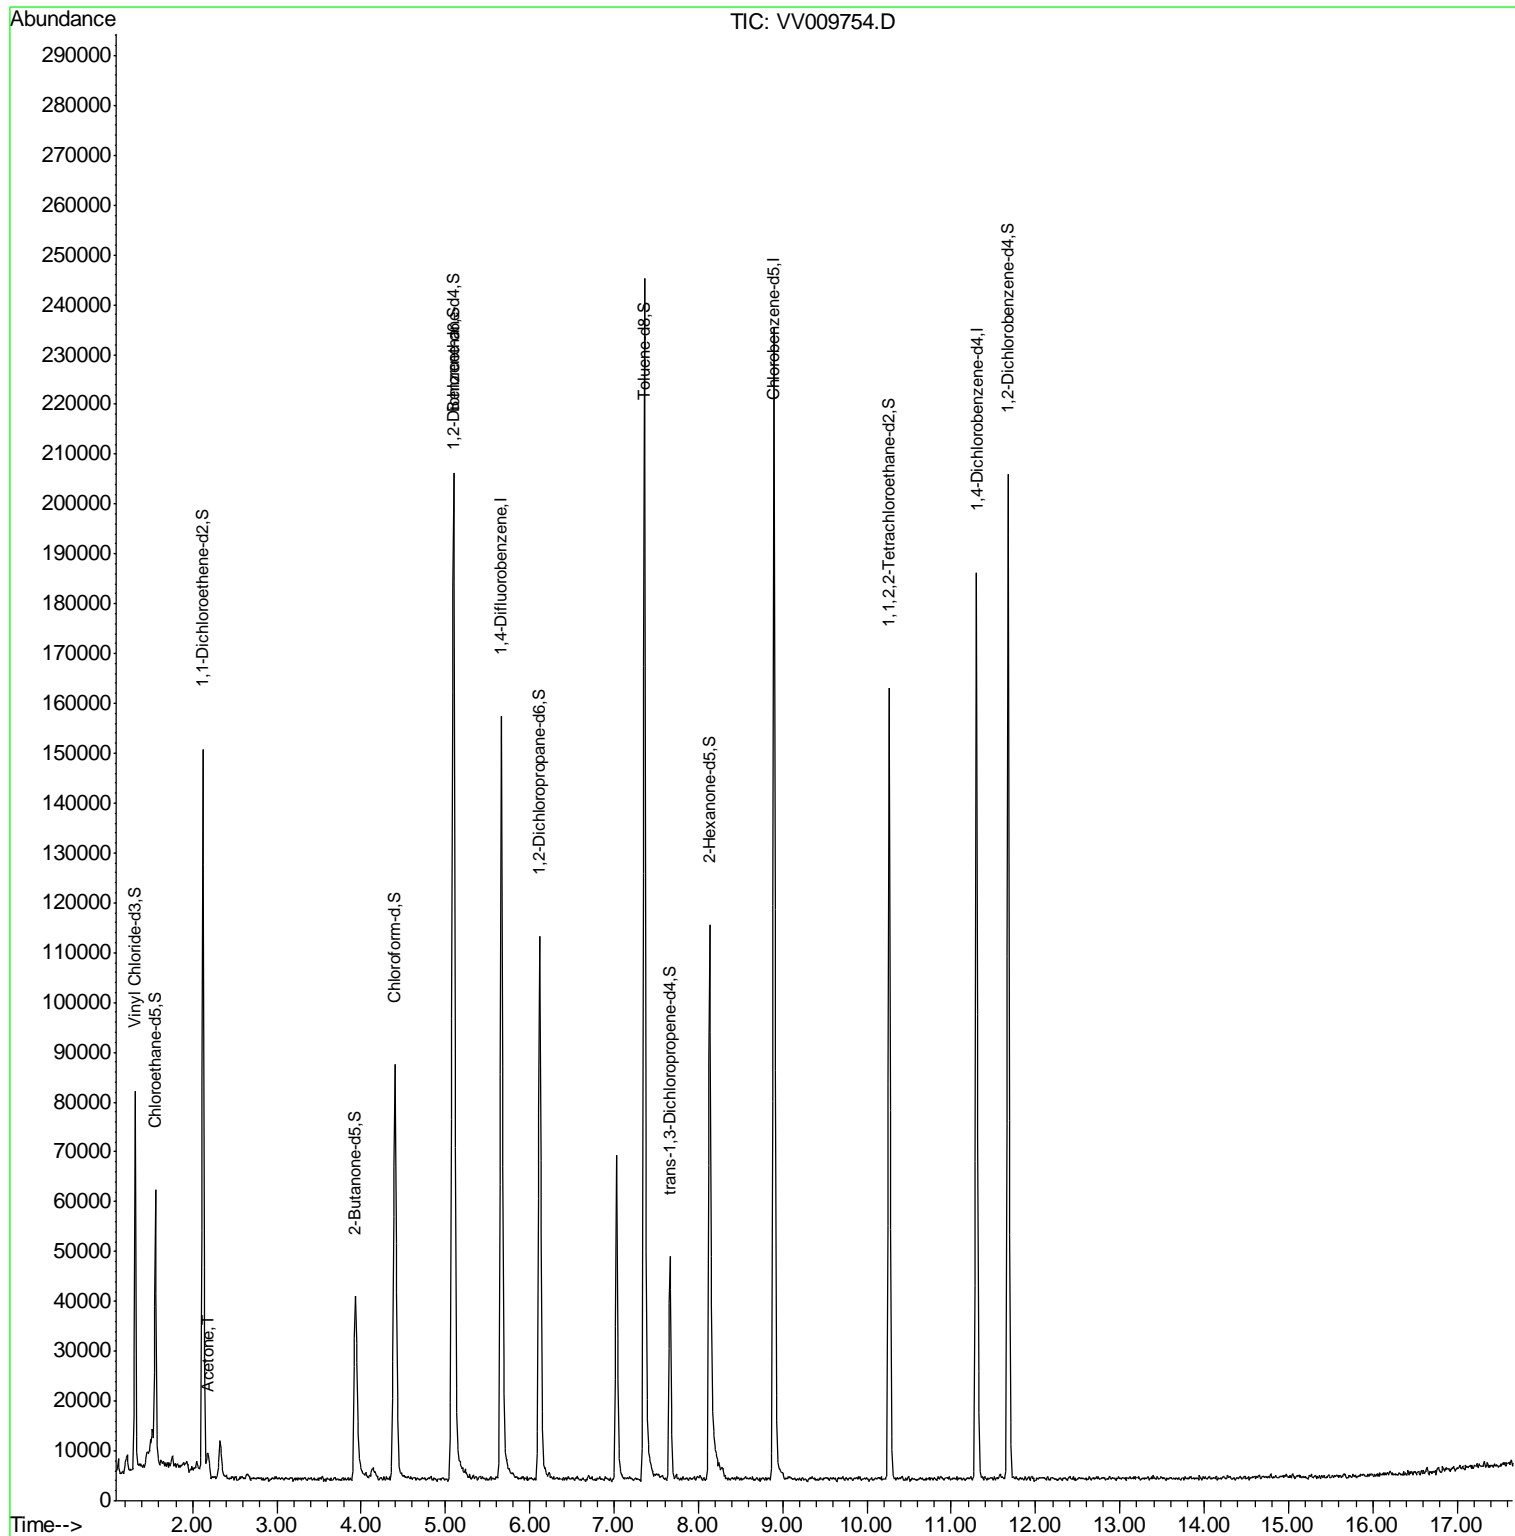

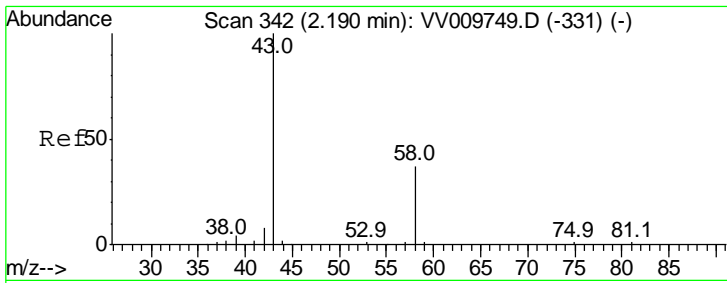

#13
 Acetone
 Concen: 6.249 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. 0.00 min
 Lab File: VV009754.D
 Acq: 18 Mar 2019 13:21

Instrument :
 MSVOA_V
 ClientSampled :
 C0991

Tot Ion: 43 Resp: 3325
 Ion Ratio Lower Upper
 43 100
 58 33.9 0.0 67.8

