

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031819\
 Data File : VV009750.D
 Acq On : 18 Mar 2019 11:43
 Operator : SY/MD
 Sample : VV0318WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	64678	66109	14.77%	1.922%
2	1.550	139	143	151	rVB	43816	42774	9.55%	1.244%
3	2.113	309	318	330	rBV	129964	182001	40.65%	5.292%
4	2.415	407	412	416	rBV2	631	592	0.13%	0.017%
5	2.505	436	440	443	rBV2	630	531	0.12%	0.015%
6	2.785	520	527	530	rBV4	1026	1204	0.27%	0.035%
7	2.994	590	592	594	rBV	379	124	0.03%	0.004%
8	3.123	630	632	635	rBV2	239	128	0.03%	0.004%
9	3.187	647	652	656	rBV	390	414	0.09%	0.012%
10	3.447	731	733	736	rBV2	305	146	0.03%	0.004%
11	3.676	802	804	806	rBV	376	237	0.05%	0.007%
12	3.933	871	884	916	rBV	30276	85840	19.17%	2.496%
13	4.164	954	956	957	rBV	388	152	0.03%	0.004%
14	4.251	980	983	990	rBV2	465	607	0.14%	0.018%
15	4.396	1010	1028	1047	rBV	72527	178921	39.97%	5.203%
16	4.656	1105	1109	1114	rVB	653	625	0.14%	0.018%
17	4.685	1116	1118	1121	rBV	397	261	0.06%	0.008%
18	4.798	1150	1153	1158	rBV2	521	527	0.12%	0.015%
19	4.981	1205	1210	1212	rBV2	700	641	0.14%	0.019%
20	5.090	1226	1244	1264	rBV2	179735	447682	100.00%	13.018%
21	5.518	1373	1377	1381	rBV2	754	760	0.17%	0.022%
22	5.659	1408	1421	1445	rBV	137396	277395	61.96%	8.067%
23	5.875	1486	1488	1490	rBV	539	325	0.07%	0.009%
24	6.055	1541	1544	1546	rBV	347	226	0.05%	0.007%
25	6.113	1548	1562	1581	rVV2	95817	195905	43.76%	5.697%
26	6.306	1619	1622	1623	rBV	207	117	0.03%	0.003%
27	6.322	1623	1627	1628	rBV2	323	230	0.05%	0.007%
28	6.354	1635	1637	1640	rBV2	426	225	0.05%	0.007%
29	6.463	1669	1671	1677	rVB	483	300	0.07%	0.009%
30	6.524	1682	1690	1692	rBV2	653	679	0.15%	0.020%
31	6.579	1703	1707	1709	rBV	488	308	0.07%	0.009%
32	6.981	1828	1832	1834	rBV2	494	427	0.10%	0.012%
33	7.026	1835	1846	1871	rVB	58245	105228	23.51%	3.060%
34	7.357	1936	1949	1966	rBV	216655	380956	85.10%	11.078%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031819\
Data File : VV009750.D
Acq On : 18 Mar 2019 11:43
Operator : SY/MD
Sample : VV0318WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK75

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Title : VOC Analysis

35	7.663	2034	2044	2062	rBV	40280	69063	15.43%	2.008%
36	7.897	2115	2117	2119	rBV2	686	349	0.08%	0.010%
37	8.074	2168	2172	2175	rBV2	507	406	0.09%	0.012%
38	8.093	2175	2178	2180	rBV	542	334	0.07%	0.010%
39	8.135	2180	2191	2213	rBV	103363	204931	45.78%	5.959%
40	8.746	2378	2381	2384	rBV	333	225	0.05%	0.007%
41	8.897	2416	2428	2444	rBV	206903	345102	77.09%	10.035%
42	9.097	2487	2490	2496	rBV	492	516	0.12%	0.015%
43	9.322	2557	2560	2562	rBV	612	417	0.09%	0.012%
44	10.103	2800	2803	2804	rBV2	334	174	0.04%	0.005%
45	10.264	2842	2853	2871	rBV	152906	245198	54.77%	7.130%
46	10.399	2892	2895	2899	rBV	431	418	0.09%	0.012%
47	10.495	2923	2925	2927	rBV	346	170	0.04%	0.005%
48	10.579	2949	2951	2952	rBV	270	128	0.03%	0.004%
49	11.164	3129	3133	3136	rBV	496	555	0.12%	0.016%
50	11.219	3147	3150	3152	rBV2	464	253	0.06%	0.007%
51	11.232	3152	3154	3155	rBV	632	296	0.07%	0.009%
52	11.299	3163	3175	3194	rBV	165610	285093	63.68%	8.290%
53	11.672	3280	3291	3308	rBV	185285	310428	69.34%	9.027%
54	12.608	3579	3582	3584	rBV	377	304	0.07%	0.009%
55	12.865	3657	3662	3664	rBV	517	514	0.11%	0.015%
56	14.174	4066	4069	4072	rBV2	783	520	0.12%	0.015%
57	16.151	4681	4684	4687	rBV2	1158	861	0.19%	0.025%


Sum of corrected areas: 3438852

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031819\
Data File : VV009750.D
Acq On : 18 Mar 2019 11:43
Operator : SY/MD
Sample : VV0318WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

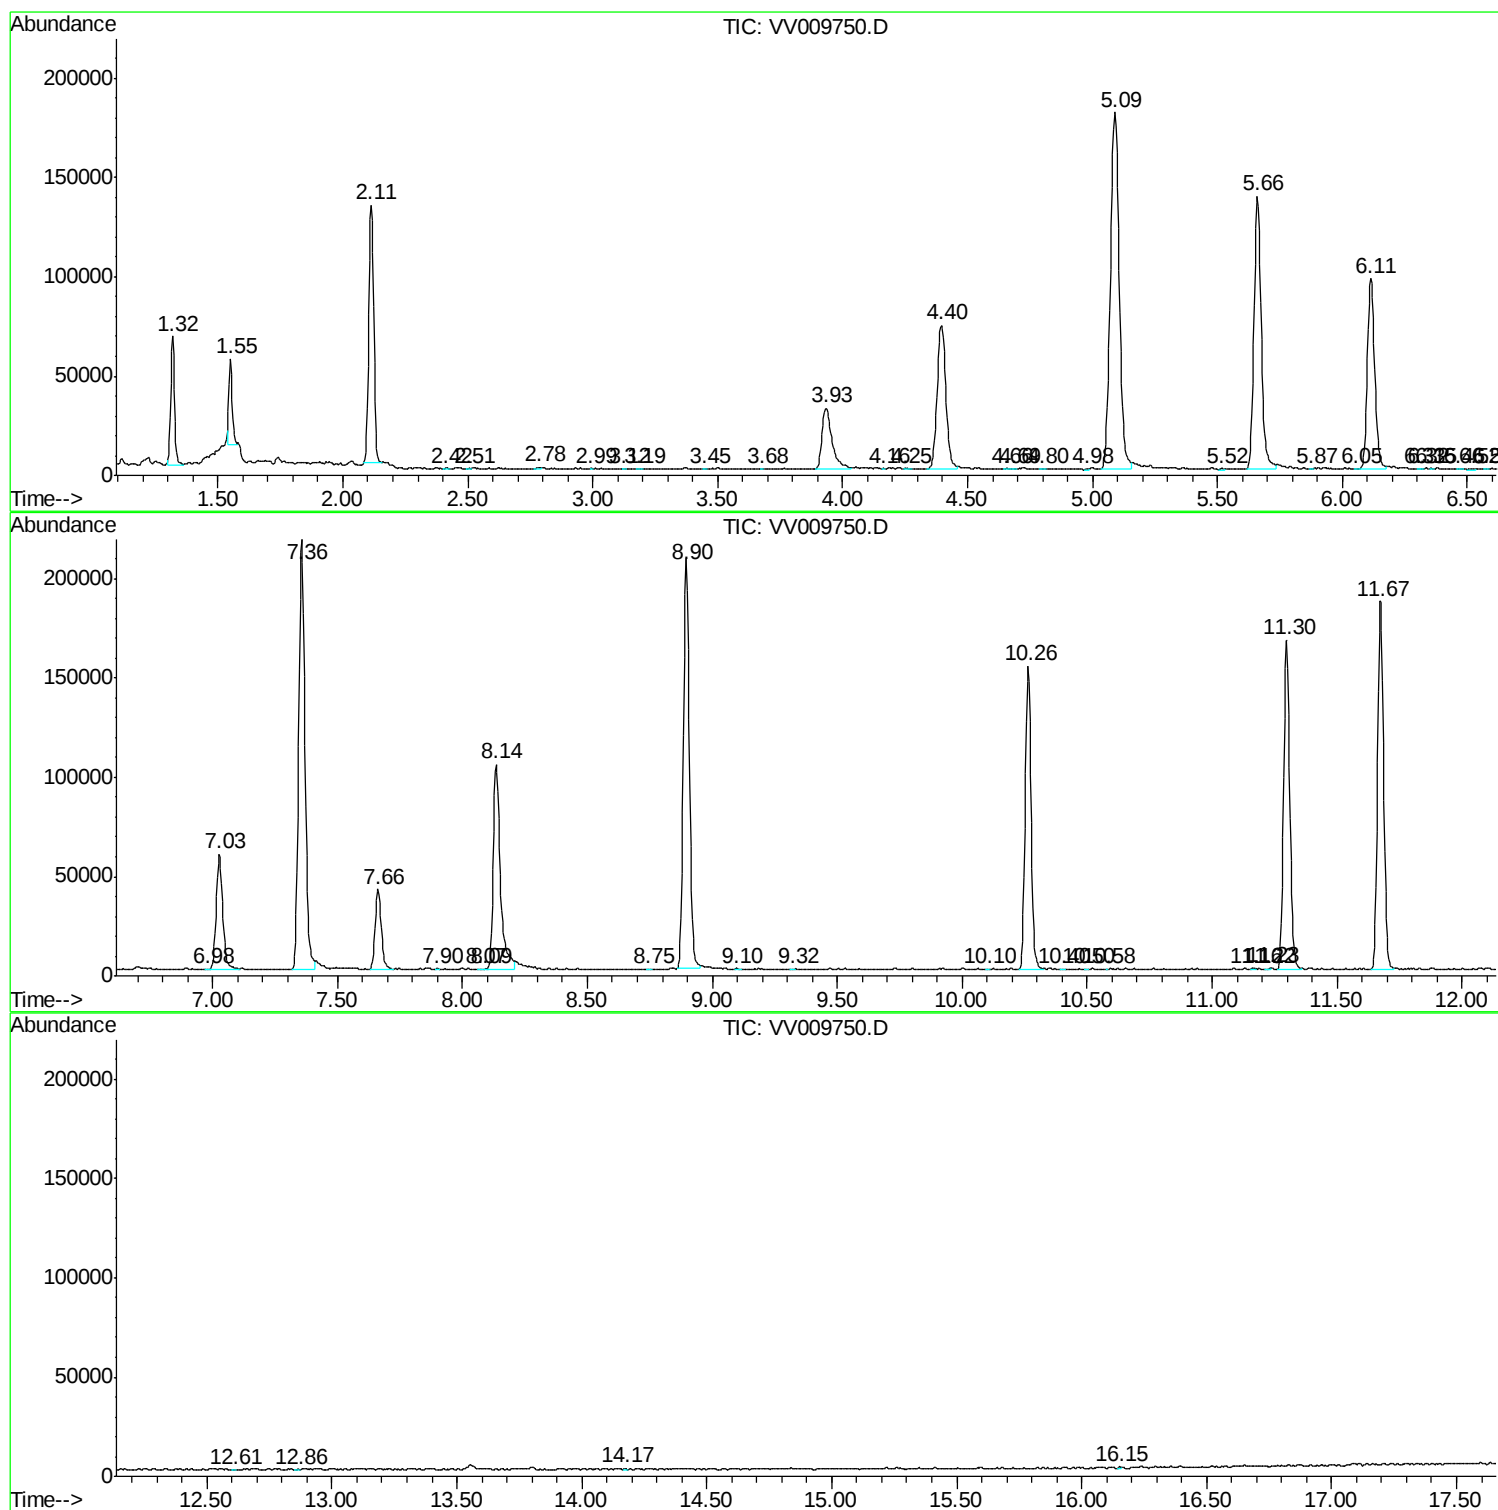

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031819\
Data File : VV009750.D
Acq On : 18 Mar 2019 11:43
Operator : SY/MD
Sample : VV0318WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031819\
Data File : VV009750.D
Acq On : 18 Mar 2019 11:43
Operator : SY/MD
Sample : VV0318WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK75

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc