


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031819\
 Data File : VV009748.D
 Acq On : 18 Mar 2019 10:35
 Operator : SY/MD
 Sample : BFB80
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB80

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 18 12:32:58 2019

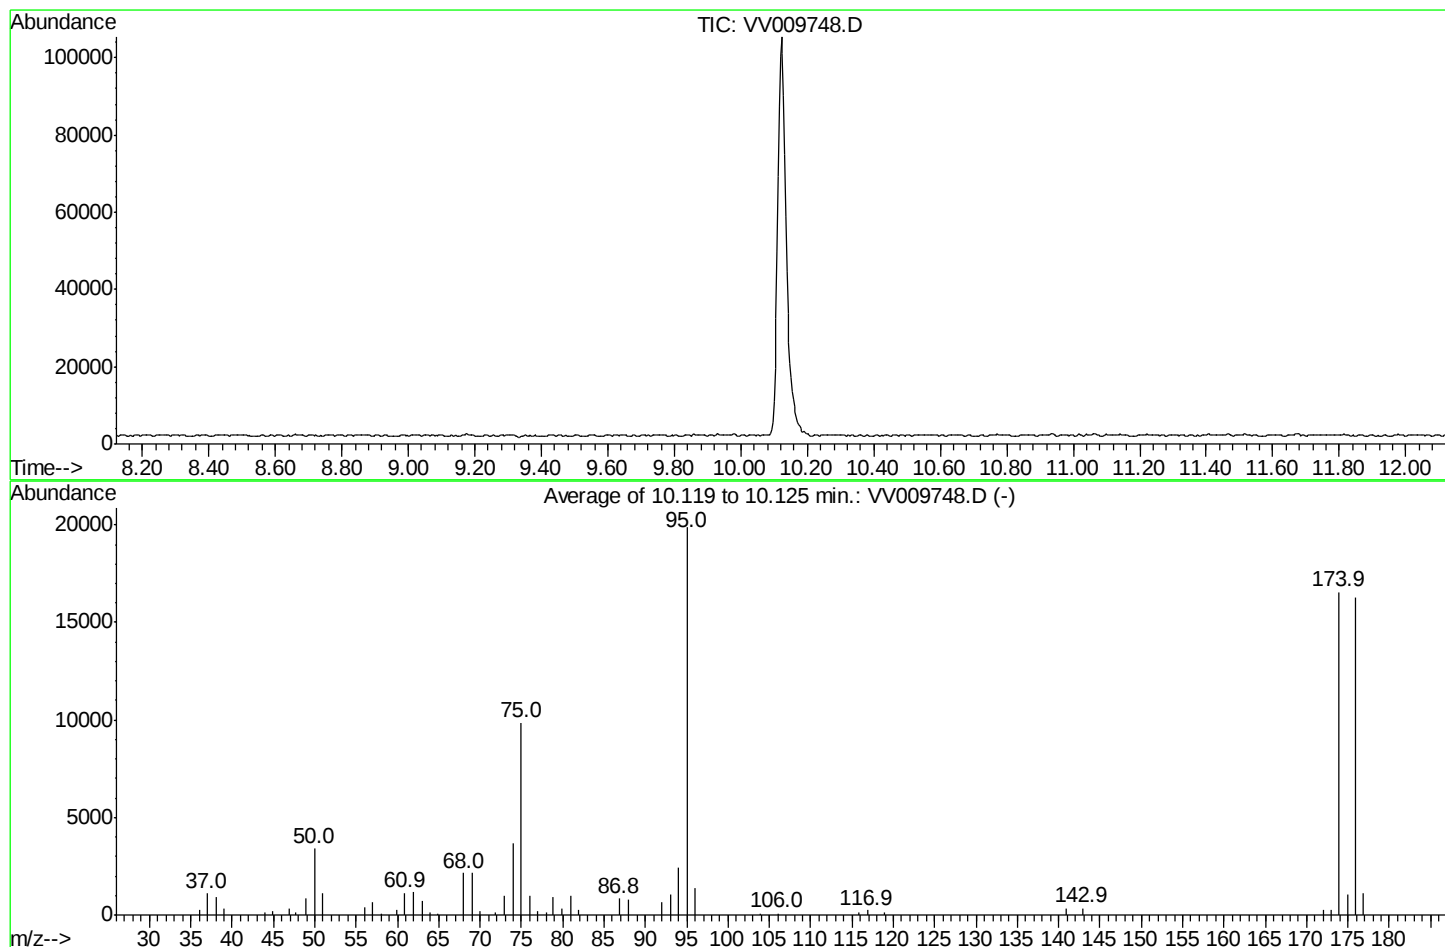

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	3385	PASS
75	95	30	80	49.7	9872	PASS
95	95	100	100	100.0	19877	PASS
96	95	5	9	7.0	1384	PASS
173	174	0.00	2	1.5	249	PASS
174	95	50	120	83.2	16540	PASS
175	174	5	9	6.4	1059	PASS
176	174	95	101	98.6	16304	PASS
177	176	5	9	6.9	1124	PASS

Scan 2797 (10.084 min): VV009748.D
BFB80

m/z	Abundance
40.00	2121.0
44.00	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	270.0
37.00	1065.0
38.00	1103.0
39.10	341.0
40.00	2040.0
43.90	372.0
44.90	187.0
46.90	363.0
47.80	127.0
48.90	781.0
50.00	3463.0
51.00	1191.0
56.00	412.0
56.90	580.0
59.90	248.0
60.90	1179.0
62.00	1220.0
63.00	677.0
64.00	175.0
68.00	2226.0
69.00	2090.0
70.00	149.0
71.80	121.0
72.90	939.0
74.00	3697.0
75.00	9573.0
76.00	1015.0
76.90	175.0
78.00	175.0
78.80	874.0
79.80	312.0
80.90	1007.0
81.80	180.0
86.80	860.0
88.00	828.0
92.00	575.0
93.00	1026.0
94.00	2273.0
95.00	19456.0
96.00	1447.0
103.90	119.0
106.00	133.0
115.80	118.0
116.90	216.0
118.90	146.0
140.80	278.0
142.90	339.0
172.10	220.0
173.00	213.0
174.00	16036.0
174.90	1079.0
175.90	15714.0
176.90	1079.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	303.0
37.00	1155.0
38.00	942.0
39.00	344.0
40.00	1950.0
44.00	384.0
44.90	194.0
46.90	321.0
47.80	123.0
48.90	876.0
50.00	3486.0
51.00	1134.0
56.00	410.0
57.00	636.0
58.00	105.0
59.90	267.0
60.90	1171.0
62.00	1213.0
62.90	731.0
64.00	143.0
64.80	122.0
68.00	2193.0
69.00	2254.0
70.00	176.0
71.80	133.0
73.00	1042.0
74.00	3770.0
75.00	10226.0
76.00	956.0
76.90	198.0
78.00	137.0
78.80	913.0
79.90	337.0
80.90	992.0
81.90	234.0
86.90	832.0
88.00	805.0
91.90	657.0
93.00	1086.0
94.00	2496.0
95.00	20368.0
96.00	1430.0
103.90	118.0
106.00	119.0
115.80	153.0
116.90	268.0
118.90	133.0
140.80	338.0
142.90	363.0
172.10	278.0
173.00	264.0
174.00	17104.0
175.00	1081.0
175.90	16776.0
176.90	1155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80

m/z	Abundance
36.00	276.0
36.90	1070.0
38.00	741.0
39.00	349.0
40.00	2012.0
44.00	389.0
44.90	183.0
46.90	217.0
47.70	122.0
49.00	842.0
50.00	3207.0
51.00	1063.0
56.00	382.0
57.00	662.0
59.90	254.0
60.90	1042.0
62.00	1038.0
62.90	733.0
63.90	114.0
64.90	165.0
68.00	2001.0
69.00	2123.0
70.00	209.0
71.80	117.0
72.90	989.0
74.00	3609.0
75.00	9817.0
76.00	899.0
76.90	173.0
78.80	888.0
79.90	352.0
80.90	911.0
81.80	286.0
86.90	838.0
88.00	679.0
91.90	679.0
93.00	1035.0
93.90	2605.0
95.00	19808.0
96.00	1276.0
115.80	131.0
116.90	255.0
118.90	152.0
140.90	387.0
142.90	333.0
172.10	262.0
173.00	271.0
173.90	16480.0
175.00	1019.0
175.90	16424.0
176.90	1139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB80