
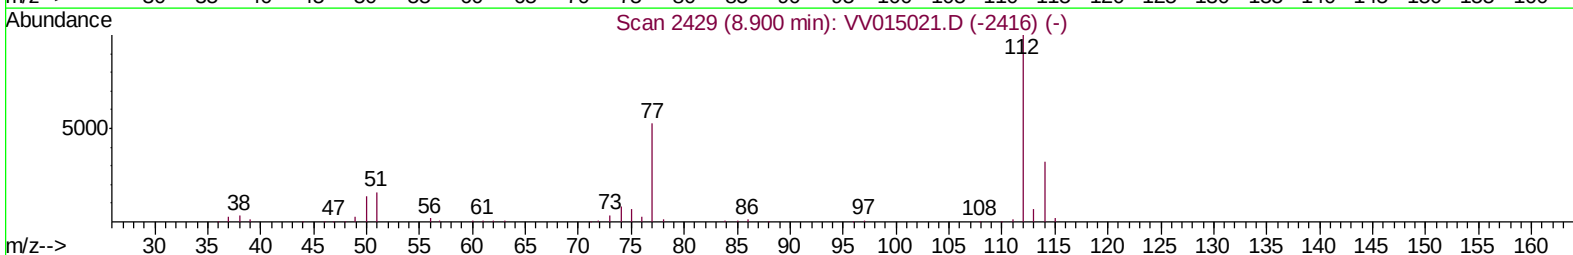
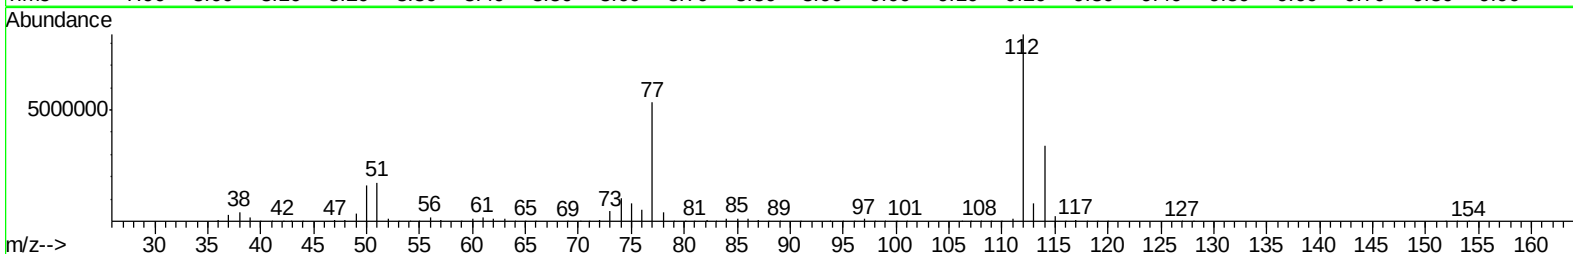


Data File : VV015037.D
Acq On : 19 Mar 2020 00:51
Operator : SY/MD
Sample : L1941-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 19 04:13:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 19 04:08:09 2020
Response via : Initial Calibration

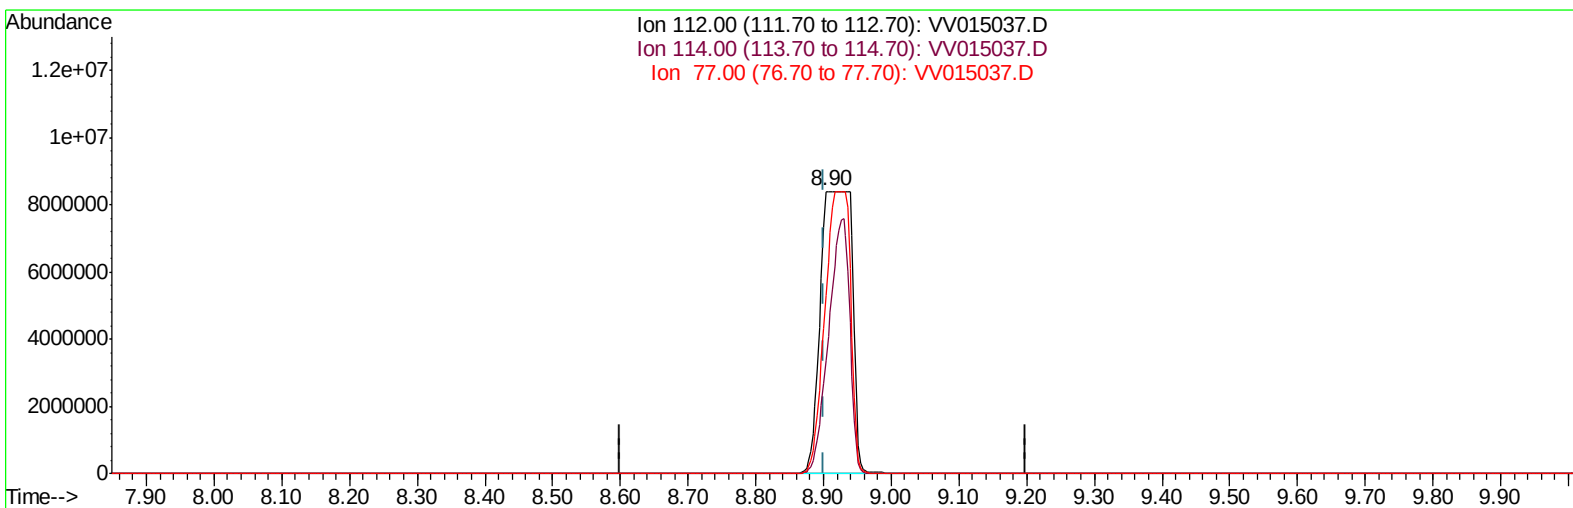

TIC: VV015037.D

(51) Chlorobenzene (T)

8.904min (+0.003) 3642.57ug/L m

response 27143389

Ion	Exp%	Act%
112.00	100	100
114.00	32.00	40.16
77.00	53.60	63.39
0.00	0.00	0.00