
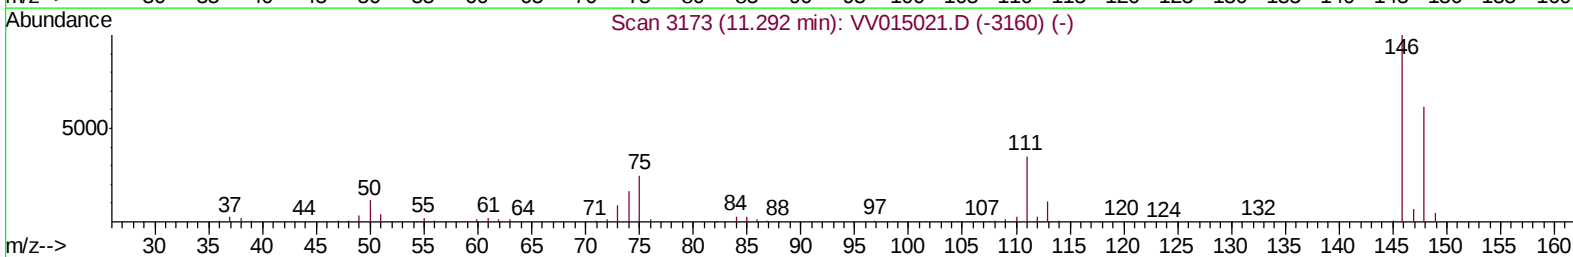
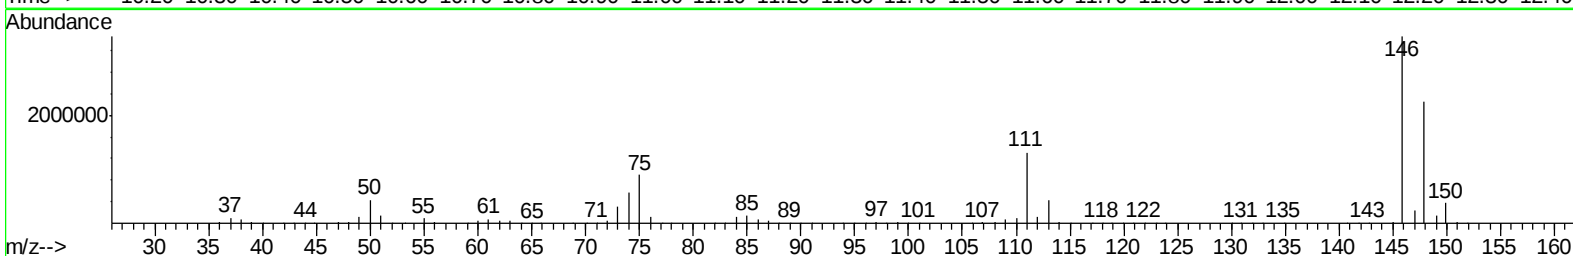


Data File : VV015037.D
Acq On : 19 Mar 2020 00:51
Operator : SY/MD
Sample : L1941-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Mar 19 04:13:21 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 19 04:08:09 2020
Response via : Initial Calibration

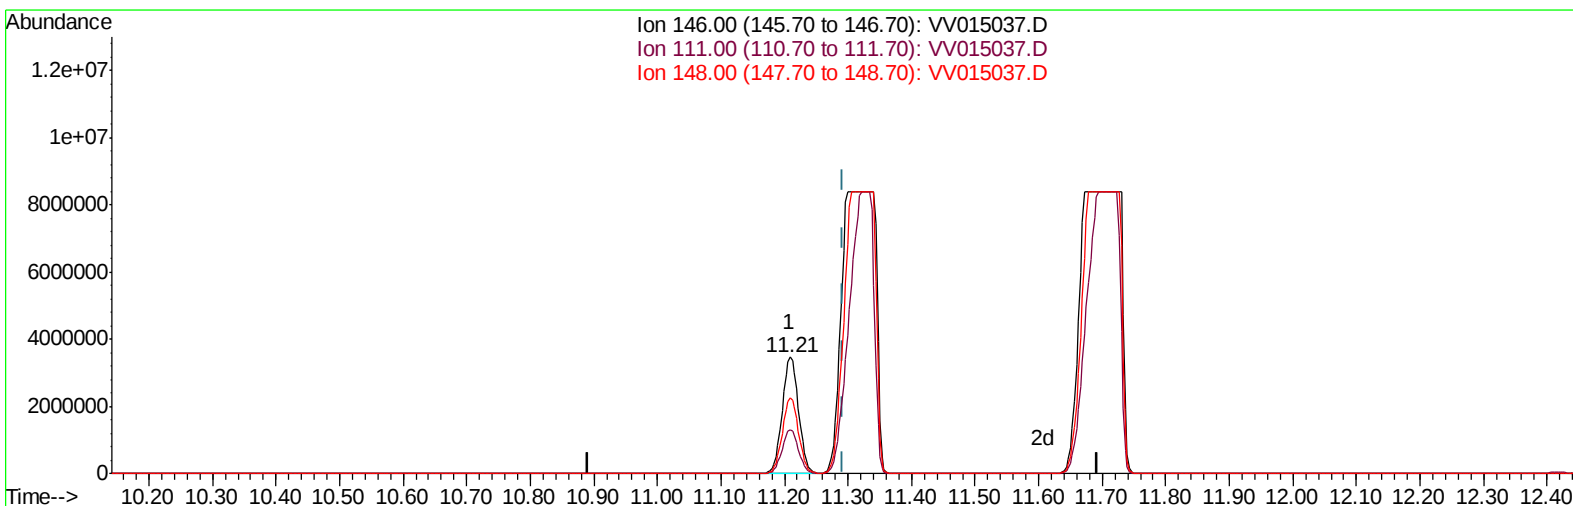

TIC: VV015037.D

(63) 1,4-Dichlorobenzene (T)

11.209min (-0.083) 798.19ug/L

response 6136312

Ion	Exp%	Act%
146.00	100	100
111.00	36.90	37.94
148.00	65.30	65.01
0.00	0.00	0.00