
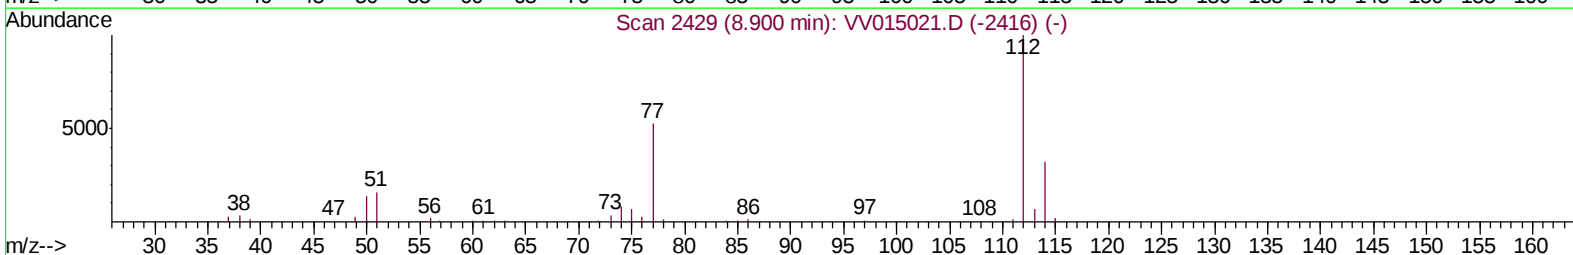
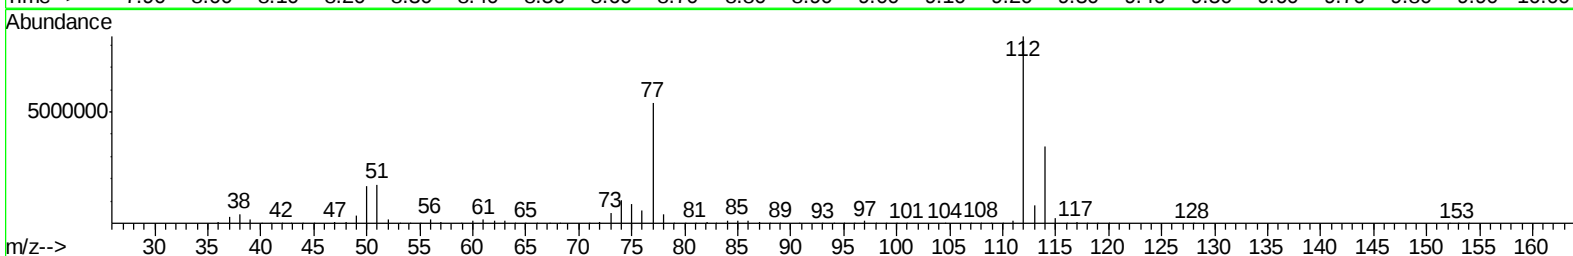


Data File : VV015039.D
Acq On : 19 Mar 2020 01:39
Operator : SY/MD
Sample : L1941-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Mar 19 04:13:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 19 04:08:09 2020
Response via : Initial Calibration

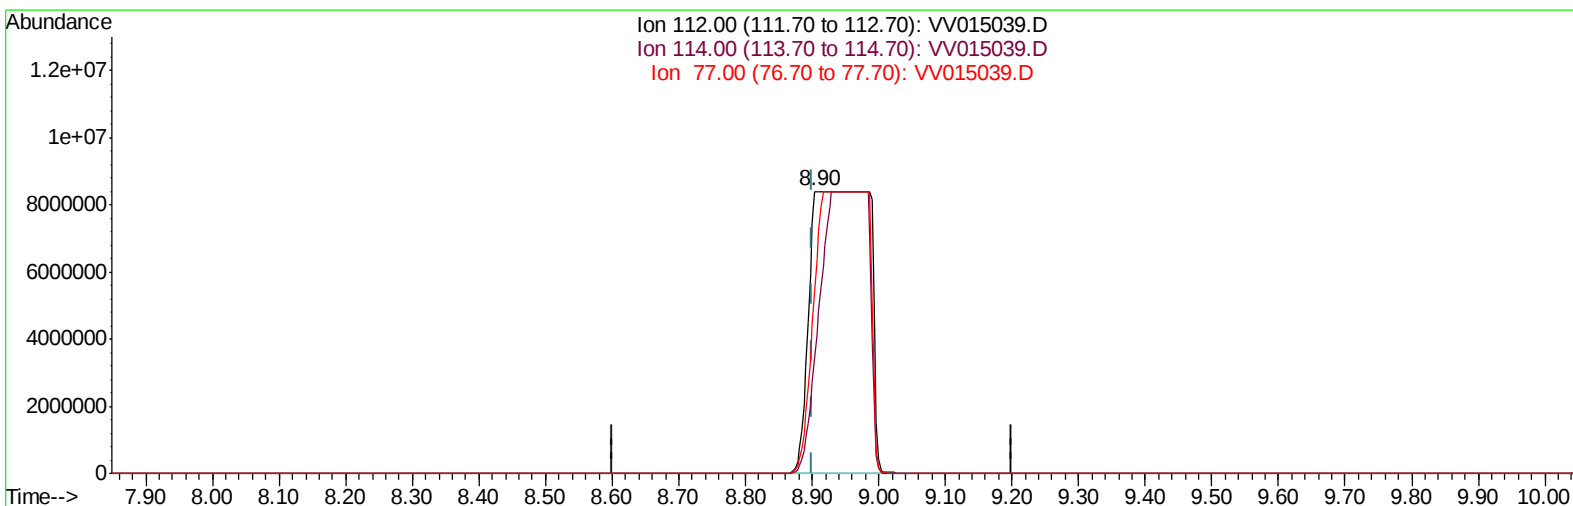

TIC: VV015039.D

(51) Chlorobenzene (T)

8.903min (+0.003) 7557.75ug/L m

response 51487226

Ion	Exp%	Act%
112.00	100	100
114.00	32.00	40.87
77.00	53.60	64.48#
0.00	0.00	0.00