
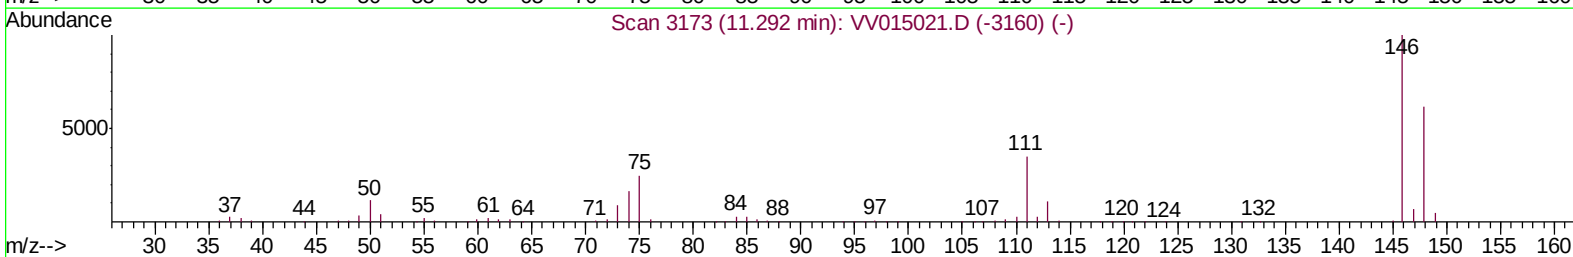
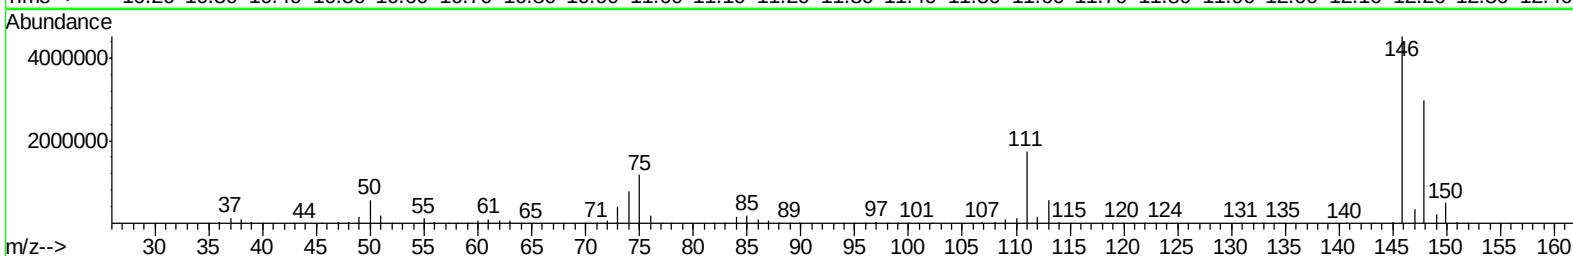


Data File : VV015041.D
Acq On : 19 Mar 2020 02:28
Operator : SY/MD
Sample : L1941-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 19 04:14:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 19 04:08:09 2020
Response via : Initial Calibration

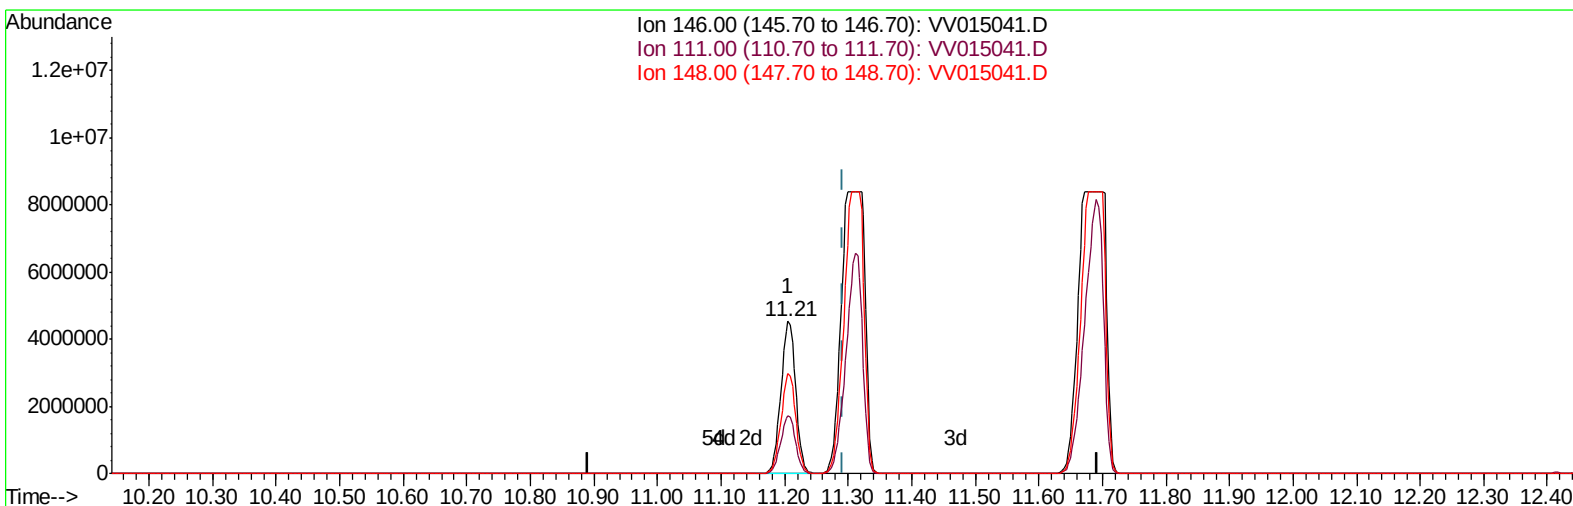

TIC: VV015041.D

(63) 1,4-Dichlorobenzene (T)

11.206min (-0.087) 1056.70ug/L

response 7273053

Ion	Exp%	Act%
146.00	100	100
111.00	36.90	38.25
148.00	65.30	65.75
0.00	0.00	0.00