
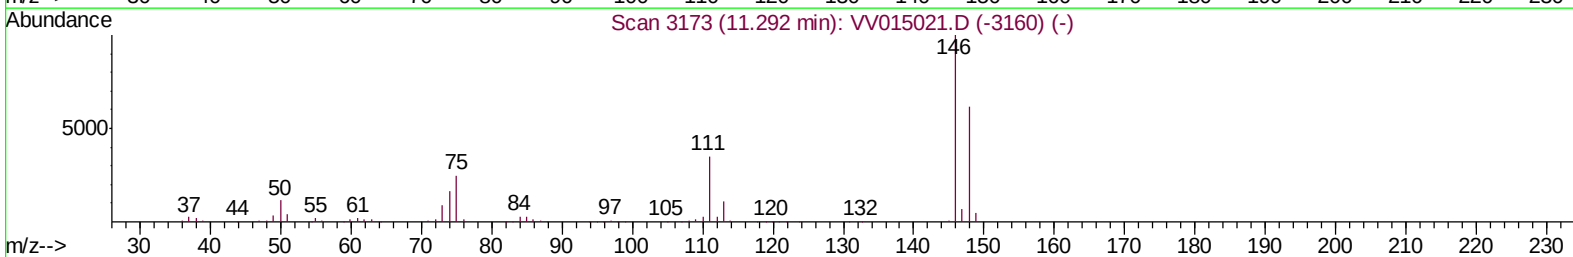
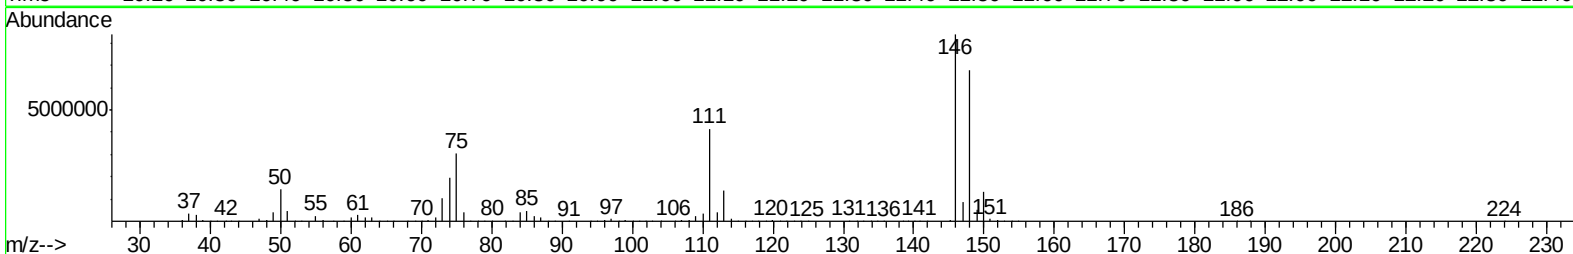


Data File : VV015041.D
Acq On : 19 Mar 2020 02:28
Operator : SY/MD
Sample : L1941-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 19 04:14:26 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 19 04:08:09 2020
Response via : Initial Calibration

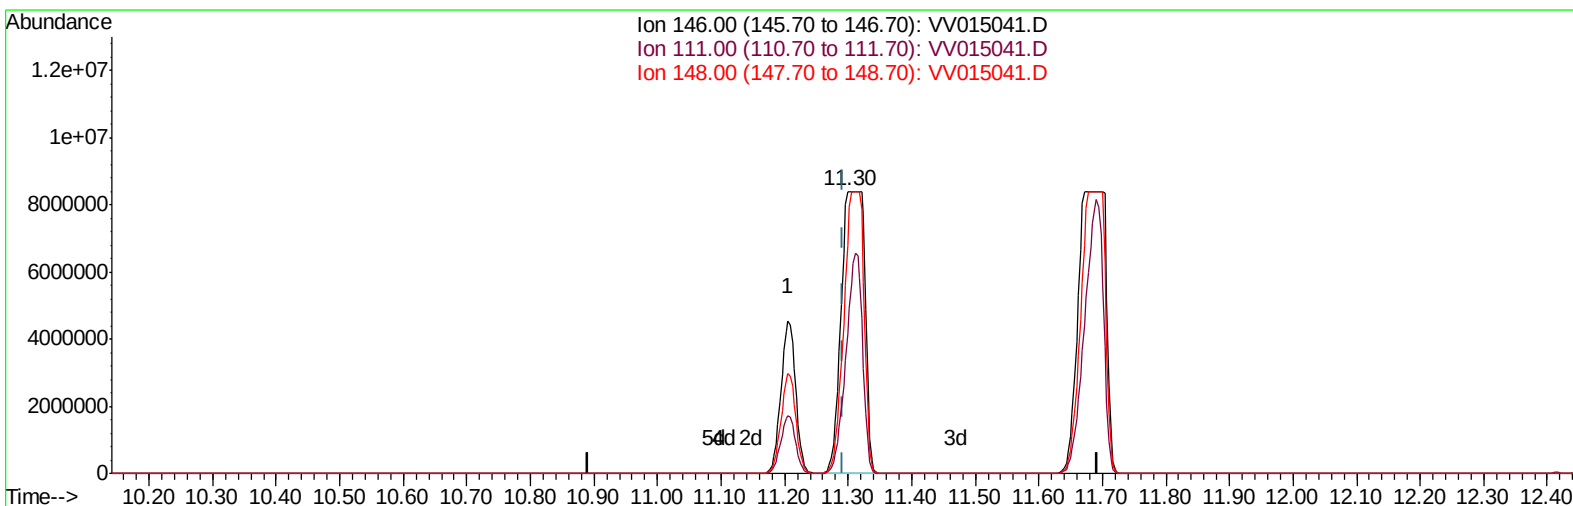

TIC: VV015041.D

(63) 1,4-Dichlorobenzene (T)

11.299min (+0.006) 3158.80ug/L m

response 21741314

Ion	Exp%	Act%
146.00	100	100
111.00	36.90	49.42#
148.00	65.30	81.09
0.00	0.00	0.00