
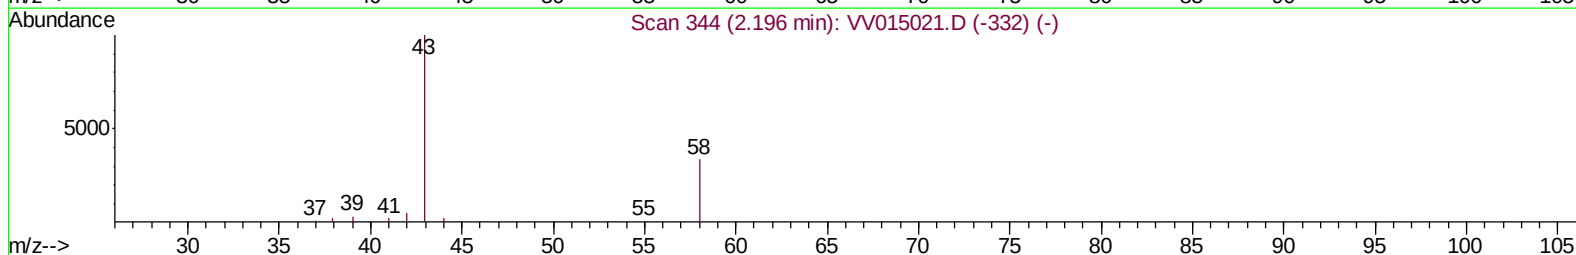
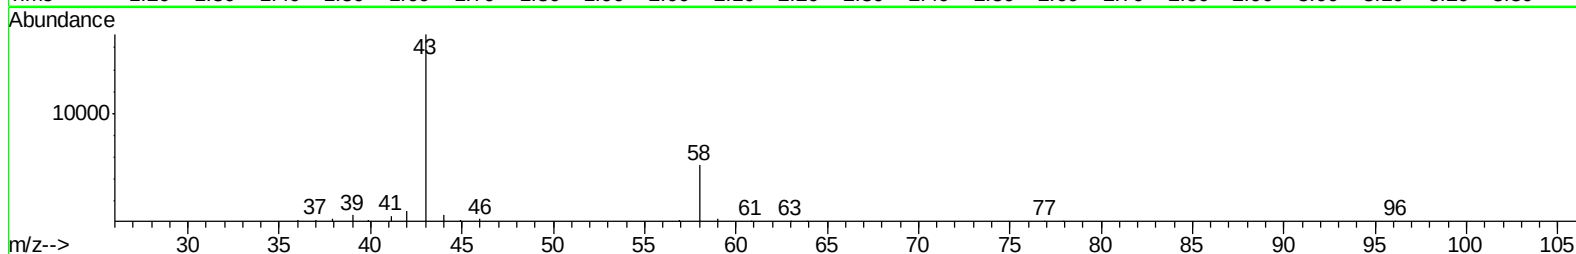


Data File : VV015043.D
Acq On : 19 Mar 2020 03:16
Operator : SY/MD
Sample : VSTDCCC050EC
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Mar 19 04:14:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 19 04:08:09 2020
Response via : Initial Calibration

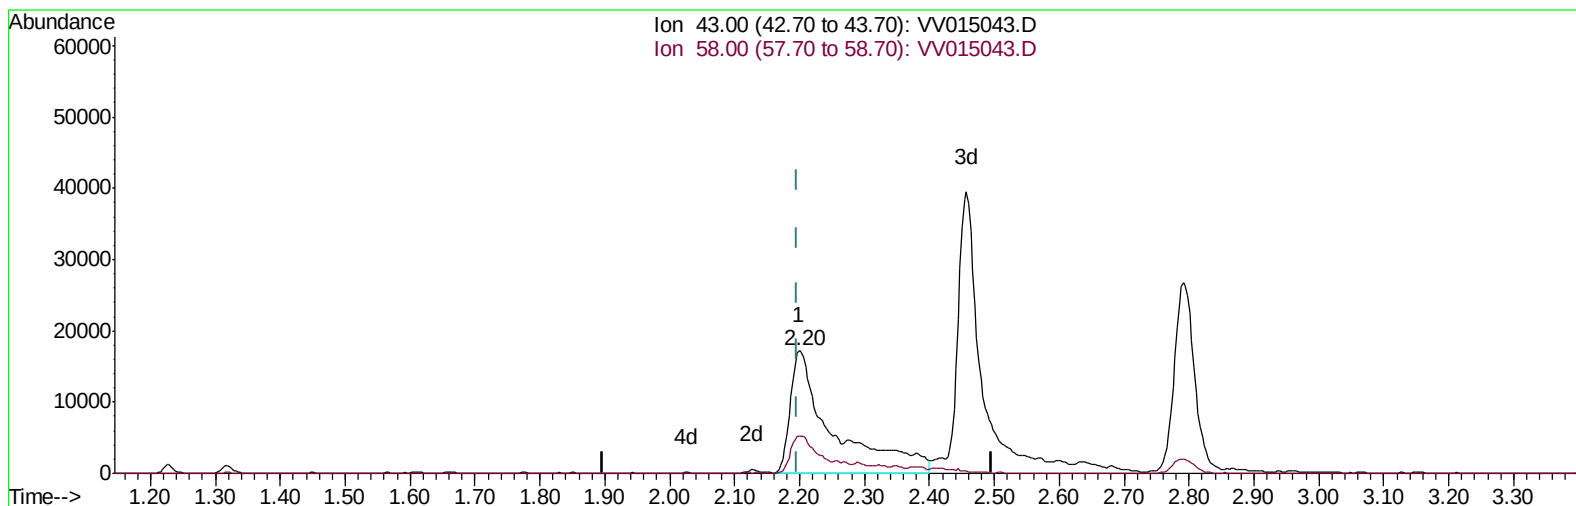

TIC: VV015043.D

(13) Acetone (T)

2.200min (+0.003) 91.46ug/L m

response 78859

Ion	Exp%	Act%
43.00	100	100
58.00	21.60	18.70
0.00	0.00	0.00
0.00	0.00	0.00