

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015023.D
 Acq On : 18 Mar 2020 19:11
 Operator : SY/MD
 Sample : L1941-11DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	37	41	50	rVB2	9817	9231	0.48%	0.086%
2	1.315	61	70	85	rBV	137408	143919	7.48%	1.342%
3	1.392	91	94	97	rBV3	1042	843	0.04%	0.008%
4	1.576	143	151	166	rVB	96896	119716	6.22%	1.116%
5	1.753	204	206	209	rVB2	745	341	0.02%	0.003%
6	1.839	231	233	236	rBV	566	379	0.02%	0.004%
7	1.868	240	242	244	rVB3	817	332	0.02%	0.003%
8	1.913	253	256	260	rBV3	799	460	0.02%	0.004%
9	1.984	276	278	281	rBV2	731	523	0.03%	0.005%
10	2.003	281	284	288	rVB2	910	752	0.04%	0.007%
11	2.077	304	307	310	rBV3	481	346	0.02%	0.003%
12	2.119	310	320	337	rVV	212649	309971	16.11%	2.890%
13	2.309	368	379	386	rBV	2041	3146	0.16%	0.029%
14	2.431	414	417	422	rVB2	413	333	0.02%	0.003%
15	2.473	427	430	435	rBV2	431	411	0.02%	0.004%
16	2.531	441	448	450	rBV2	592	613	0.03%	0.006%
17	2.640	476	482	490	rVV3	1219	1911	0.10%	0.018%
18	2.765	516	521	522	rBV2	503	346	0.02%	0.003%
19	3.193	652	654	659	rVB	451	323	0.02%	0.003%
20	3.219	659	662	665	rBV2	386	342	0.02%	0.003%
21	3.254	667	673	676	rVV2	229	270	0.01%	0.003%
22	3.569	765	771	775	rBV	223	278	0.01%	0.003%
23	3.933	869	884	917	rBV	49785	212143	11.03%	1.978%
24	4.376	1004	1022	1046	rBV	187258	461891	24.01%	4.306%
25	4.550	1074	1076	1079	rBV2	409	292	0.02%	0.003%
26	4.601	1090	1092	1096	rVB2	383	274	0.01%	0.003%
27	4.634	1100	1102	1105	rVB	537	309	0.02%	0.003%
28	4.662	1105	1111	1114	rBV2	294	373	0.02%	0.003%
29	4.707	1122	1125	1127	rBV	449	261	0.01%	0.002%
30	4.958	1199	1203	1208	rVV3	349	320	0.02%	0.003%
31	5.074	1220	1239	1264	rBV2	458289	1154408	60.00%	10.763%
32	5.248	1290	1293	1294	rBV2	468	279	0.01%	0.003%
33	5.309	1308	1312	1313	rBV2	476	326	0.02%	0.003%
34	5.334	1318	1320	1324	rVB	491	275	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015023.D
 Acq On : 18 Mar 2020 19:11
 Operator : SY/MD
 Sample : L1941-11DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

35	5.367	1326	1330	1334	rBV	373	330	0.02%	0.003%
36	5.492	1365	1369	1373	rBV3	679	657	0.03%	0.006%
37	5.643	1400	1416	1435	rBV	385879	759749	39.49%	7.083%
38	5.814	1466	1469	1475	rVB	400	305	0.02%	0.003%
39	5.929	1497	1505	1515	rVB8	1886	3685	0.19%	0.034%
40	6.096	1542	1557	1583	rBV	246289	504697	26.23%	4.705%
41	6.225	1593	1597	1599	rBV3	400	376	0.02%	0.004%
42	6.347	1631	1635	1638	rVV2	403	322	0.02%	0.003%
43	6.534	1688	1693	1696	rBV2	346	380	0.02%	0.004%
44	6.649	1722	1729	1732	rBV2	645	746	0.04%	0.007%
45	6.720	1744	1751	1756	rBV3	408	455	0.02%	0.004%
46	7.010	1826	1841	1859	rBV	143244	259316	13.48%	2.418%
47	7.254	1911	1917	1922	rBV2	553	509	0.03%	0.005%
48	7.276	1922	1924	1929	rBV2	292	263	0.01%	0.002%
49	7.338	1930	1943	1975	rBV	586849	1019010	52.96%	9.500%
50	7.508	1994	1996	1999	rBV	413	346	0.02%	0.003%
51	7.643	2027	2038	2059	rVV	101166	173904	9.04%	1.621%
52	7.994	2143	2147	2155	rVB4	1085	1116	0.06%	0.010%
53	8.119	2174	2186	2223	rBV2	259370	579809	30.14%	5.406%
54	8.338	2251	2254	2257	rVB2	474	277	0.01%	0.003%
55	8.360	2257	2261	2263	rVB2	382	262	0.01%	0.002%
56	8.386	2266	2269	2276	rVV4	344	311	0.02%	0.003%
57	8.489	2299	2301	2307	rVB	338	304	0.02%	0.003%
58	8.537	2312	2316	2319	rBV2	393	359	0.02%	0.003%
59	8.701	2365	2367	2372	rVV2	383	305	0.02%	0.003%
60	8.781	2389	2392	2402	rVB	372	315	0.02%	0.003%
61	8.871	2407	2420	2449	rBV2	590643	1213346	63.06%	11.312%
62	9.109	2489	2494	2498	rBV3	575	536	0.03%	0.005%
63	9.167	2503	2512	2518	rBV4	912	1458	0.08%	0.014%
64	9.225	2522	2530	2531	rBV2	335	350	0.02%	0.003%
65	9.251	2534	2538	2543	rVB2	362	329	0.02%	0.003%
66	9.566	2632	2636	2639	rBV3	634	522	0.03%	0.005%
67	9.588	2639	2643	2647	rVB4	750	752	0.04%	0.007%
68	9.952	2749	2756	2761	rBV3	643	868	0.05%	0.008%
69	10.238	2832	2845	2863	rVV	368529	582180	30.26%	5.428%
70	10.524	2931	2934	2939	rBV2	416	334	0.02%	0.003%
71	10.559	2939	2945	2955	rVB3	801	1081	0.06%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015023.D
 Acq On : 18 Mar 2020 19:11
 Operator : SY/MD
 Sample : L1941-11DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

72	10.730	2990	2998	3000	rVV2	350	300	0.02%	0.003%
73	10.839	3029	3032	3036	rVB2	514	329	0.02%	0.003%
74	10.939	3057	3063	3065	rVV2	1131	1139	0.06%	0.011%
75	11.103	3106	3114	3118	rBV	379	463	0.02%	0.004%
76	11.202	3136	3145	3154	rVV	18854	28824	1.50%	0.269%
77	11.270	3154	3166	3193	rVB	614719	1038246	53.96%	9.680%
78	11.399	3205	3206	3212	rVB	351	263	0.01%	0.002%
79	11.656	3269	3286	3310	rBV2	804088	1924002	100.00%	17.938%
80	11.884	3353	3357	3359	rBV3	320	291	0.02%	0.003%
81	12.225	3458	3463	3467	rBV2	395	407	0.02%	0.004%
82	12.312	3488	3490	3495	rVB3	354	322	0.02%	0.003%
83	12.421	3521	3524	3532	rVB5	739	917	0.05%	0.009%
84	12.672	3592	3602	3611	rVB7	3364	5308	0.28%	0.049%
85	12.849	3653	3657	3660	rBV2	351	283	0.01%	0.003%
86	13.283	3777	3792	3807	rBV	97667	152659	7.93%	1.423%
87	13.363	3815	3817	3822	rVB2	492	286	0.01%	0.003%
88	13.527	3862	3868	3879	rVB4	1872	2584	0.13%	0.024%
89	13.662	3907	3910	3914	rVB2	386	283	0.01%	0.003%
90	13.768	3933	3943	3957	rVB2	18964	28362	1.47%	0.264%
91	13.958	3998	4002	4006	rVB3	466	441	0.02%	0.004%
92	14.289	4102	4105	4107	rBV2	384	260	0.01%	0.002%
93	14.434	4147	4150	4153	rBV4	570	470	0.02%	0.004%
94	14.469	4157	4161	4162	rBV2	377	286	0.01%	0.003%
95	14.598	4195	4201	4204	rBV4	761	950	0.05%	0.009%
96	14.649	4214	4217	4219	rBV2	435	292	0.02%	0.003%
97	14.993	4320	4324	4329	rBV6	852	751	0.04%	0.007%
98	15.070	4347	4348	4352	rBV3	499	353	0.02%	0.003%
99	15.093	4353	4355	4357	rVB3	693	301	0.02%	0.003%
100	15.791	4569	4572	4574	rBV2	1392	958	0.05%	0.009%


Sum of corrected areas: 10726131

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015023.D
Acq On : 18 Mar 2020 19:11
Operator : SY/MD
Sample : L1941-11DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

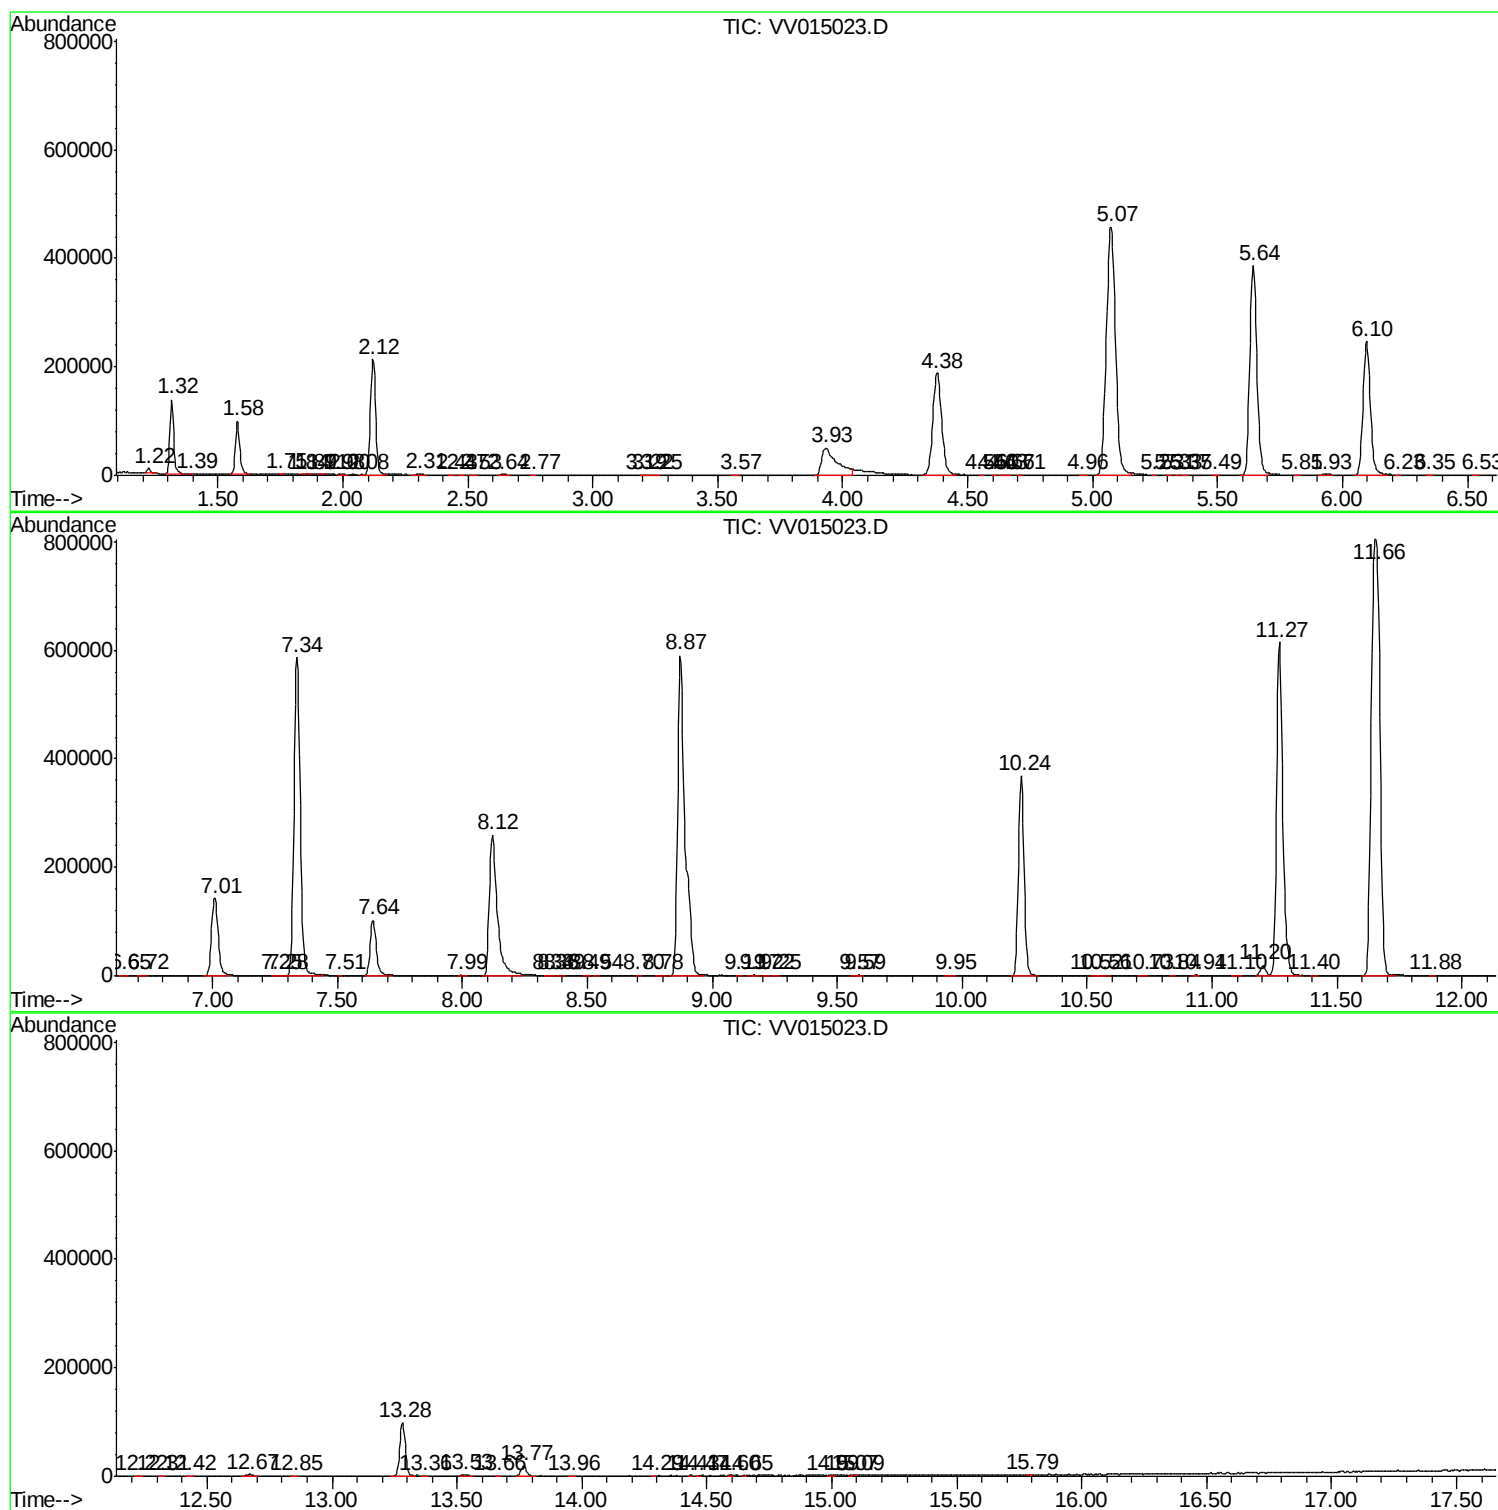

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015023.D
Acq On : 18 Mar 2020 19:11
Operator : SY/MD
Sample : L1941-11DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031820\
Data File : VV015023.D
Acq On : 18 Mar 2020 19:11
Operator : SY/MD
Sample : L1941-11DL 50X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DC2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc