

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015025.D
 Acq On : 18 Mar 2020 20:00
 Operator : SY/MD
 Sample : L1941-04DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	88	rVB	132692	139161	11.55%	1.431%
2	1.579	144	152	170	rVB	93950	120161	9.97%	1.236%
3	2.119	309	320	342	rVB	205142	299825	24.89%	3.083%
4	2.306	373	378	384	rBV2	1767	2152	0.18%	0.022%
5	2.601	467	470	473	rBV4	389	315	0.03%	0.003%
6	3.103	624	626	635	rVB3	234	238	0.02%	0.002%
7	3.135	635	636	637	rVB	154	30	0.00%	0.000%
8	3.151	637	641	643	rBV	295	207	0.02%	0.002%
9	3.203	655	657	661	rBV	179	91	0.01%	0.001%
10	3.315	689	692	695	rBV2	209	151	0.01%	0.002%
11	3.492	744	747	750	rBV	169	144	0.01%	0.001%
12	3.508	750	752	755	rVB	259	140	0.01%	0.001%
13	3.527	755	758	759	rBV	253	165	0.01%	0.002%
14	3.791	837	840	844	rVB2	271	182	0.02%	0.002%
15	3.820	846	849	850	rBV	179	85	0.01%	0.001%
16	3.875	860	866	868	rBV	262	323	0.03%	0.003%
17	3.933	872	884	922	rBV	49554	225594	18.73%	2.320%
18	4.379	1005	1023	1047	rBV	187176	464502	38.56%	4.777%
19	4.650	1106	1107	1108	rBV	221	71	0.01%	0.001%
20	4.720	1127	1129	1131	rBV	225	71	0.01%	0.001%
21	4.842	1164	1167	1169	rBV	436	311	0.03%	0.003%
22	4.936	1194	1196	1199	rVB2	353	129	0.01%	0.001%
23	5.074	1220	1239	1250	rBV2	460561	1174006	97.45%	12.073%
24	5.434	1347	1351	1358	rBV3	514	669	0.06%	0.007%
25	5.537	1380	1383	1386	rBV2	205	149	0.01%	0.002%
26	5.556	1386	1389	1390	rBV2	280	128	0.01%	0.001%
27	5.643	1400	1416	1440	rBV	373457	737850	61.25%	7.588%
28	5.868	1484	1486	1487	rVB	284	69	0.01%	0.001%
29	6.019	1531	1533	1537	rBV	305	248	0.02%	0.003%
30	6.096	1543	1557	1585	rBV	248342	512921	42.58%	5.275%
31	6.283	1612	1615	1619	rBV3	337	245	0.02%	0.003%
32	6.379	1643	1645	1648	rVB	300	132	0.01%	0.001%
33	6.479	1674	1676	1679	rBV2	303	193	0.02%	0.002%
34	6.637	1722	1725	1726	rBV2	518	312	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015025.D
 Acq On : 18 Mar 2020 20:00
 Operator : SY/MD
 Sample : L1941-04DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

35	6.868	1794	1797	1801	rBV2	364	226	0.02%	0.002%
36	6.926	1812	1815	1818	rBV	424	297	0.02%	0.003%
37	7.006	1828	1840	1866	rBV2	144845	262330	21.77%	2.698%
38	7.148	1882	1884	1887	rBV2	338	175	0.01%	0.002%
39	7.238	1909	1912	1913	rBV	335	170	0.01%	0.002%
40	7.264	1917	1920	1924	rBV4	476	419	0.03%	0.004%
41	7.338	1930	1943	1975	rBV	582170	1018337	84.53%	10.472%
42	7.588	2019	2021	2025	rBV	241	202	0.02%	0.002%
43	7.643	2027	2038	2064	rVB	100176	174455	14.48%	1.794%
44	8.119	2171	2186	2220	rBV	278959	598302	49.66%	6.153%
45	8.601	2334	2336	2337	rBV	164	57	0.00%	0.001%
46	8.624	2341	2343	2344	rBV	346	143	0.01%	0.001%
47	8.871	2408	2420	2426	rBV	573434	968145	80.36%	9.956%
48	9.148	2504	2506	2508	rBV	377	222	0.02%	0.002%
49	9.251	2534	2538	2540	rBV2	294	130	0.01%	0.001%
50	9.357	2569	2571	2573	rBV2	352	160	0.01%	0.002%
51	9.399	2581	2584	2585	rBV	255	153	0.01%	0.002%
52	9.563	2631	2635	2637	rBV2	628	560	0.05%	0.006%
53	10.238	2832	2845	2867	rBV	384981	600183	49.82%	6.172%
54	10.559	2940	2945	2947	rBV3	744	635	0.05%	0.007%
55	10.707	2989	2991	2995	rBV2	194	77	0.01%	0.001%
56	10.894	3046	3049	3050	rBV	134	73	0.01%	0.001%
57	10.903	3050	3052	3055	rVB	220	79	0.01%	0.001%
58	10.929	3057	3060	3061	rBV	497	276	0.02%	0.003%
59	11.202	3137	3145	3154	rBV2	10440	15467	1.28%	0.159%
60	11.270	3154	3166	3196	rVB2	594936	1156612	96.00%	11.894%
61	11.646	3270	3283	3307	rBV2	642125	1204745	100.00%	12.389%
62	11.942	3372	3375	3378	rVB	381	210	0.02%	0.002%
63	12.061	3411	3412	3413	rBV	248	59	0.00%	0.001%
64	12.260	3472	3474	3477	rBV	335	219	0.02%	0.002%
65	12.575	3570	3572	3575	rBV3	373	201	0.02%	0.002%
66	12.804	3641	3643	3645	rBV3	257	104	0.01%	0.001%
67	12.874	3664	3665	3668	rBV	285	185	0.02%	0.002%
68	13.283	3783	3792	3808	rVB3	21006	33518	2.78%	0.345%
69	13.765	3935	3942	3951	rBV5	4079	5562	0.46%	0.057%
70	14.267	4096	4098	4104	rVB3	558	352	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015025.D
Acq On : 18 Mar 2020 20:00
Operator : SY/MD
Sample : L1941-04DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB4DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Title : VOC Analysis


Sum of corrected areas: 9724010

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015025.D
Acq On : 18 Mar 2020 20:00
Operator : SY/MD
Sample : L1941-04DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

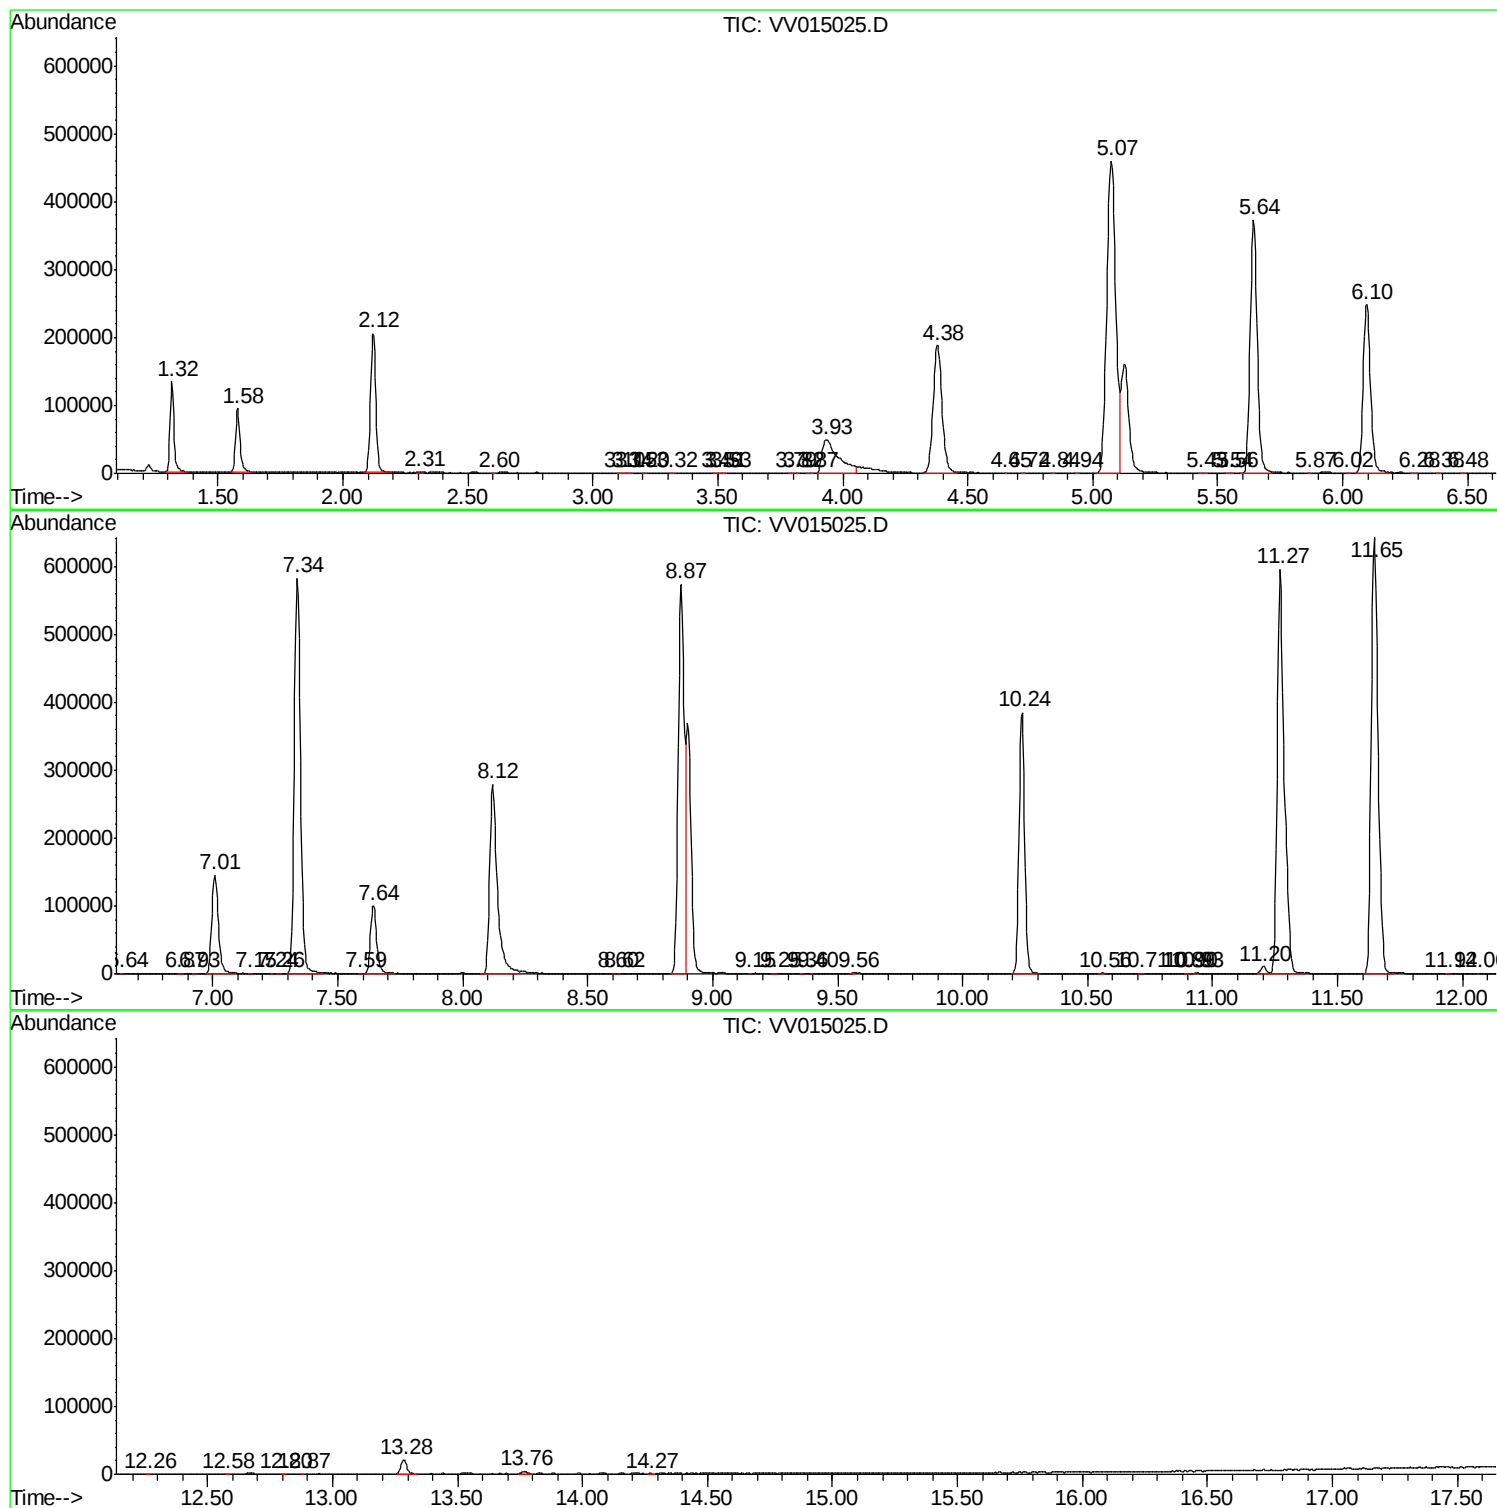

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015025.D
Acq On : 18 Mar 2020 20:00
Operator : SY/MD
Sample : L1941-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031820\
Data File : VV015025.D
Acq On : 18 Mar 2020 20:00
Operator : SY/MD
Sample : L1941-04DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DB4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc