

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015027.D
 Acq On : 18 Mar 2020 20:48
 Operator : SY/MD
 Sample : L1941-06DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	37	41	48	rVB2	10151	10106	0.39%	0.079%
2	1.315	63	70	90	rVB	132043	141366	5.45%	1.107%
3	1.576	144	151	169	rVB	94932	118250	4.55%	0.926%
4	2.119	309	320	346	rBV	212246	304363	11.72%	2.383%
5	2.579	459	463	465	rBV	401	328	0.01%	0.003%
6	2.717	504	506	509	rVB	317	183	0.01%	0.001%
7	3.116	626	630	633	rBV2	220	227	0.01%	0.002%
8	3.132	633	635	636	rVV	241	78	0.00%	0.001%
9	3.190	652	653	657	rBV	253	159	0.01%	0.001%
10	3.270	674	678	682	rBV	204	250	0.01%	0.002%
11	3.605	780	782	785	rBV	168	80	0.00%	0.001%
12	3.820	847	849	850	rBV	304	145	0.01%	0.001%
13	3.855	857	860	862	rBV2	256	140	0.01%	0.001%
14	3.933	872	884	913	rBV	45004	184349	7.10%	1.444%
15	4.376	1006	1022	1047	rBV2	184174	454988	17.53%	3.563%
16	4.621	1092	1098	1099	rBV2	300	288	0.01%	0.002%
17	4.643	1103	1105	1110	rVB2	344	234	0.01%	0.002%
18	4.669	1110	1113	1116	rBV2	244	161	0.01%	0.001%
19	4.769	1142	1144	1145	rBV	200	96	0.00%	0.001%
20	5.074	1221	1239	1266	rBV2	455906	1149102	44.26%	8.998%
21	5.344	1321	1323	1324	rBV2	197	63	0.00%	0.000%
22	5.383	1333	1335	1337	rBV	308	164	0.01%	0.001%
23	5.408	1341	1343	1347	rVB	289	169	0.01%	0.001%
24	5.460	1357	1359	1360	rBV	218	64	0.00%	0.001%
25	5.489	1366	1368	1369	rBV	203	79	0.00%	0.001%
26	5.531	1379	1381	1382	rBV	188	52	0.00%	0.000%
27	5.589	1395	1399	1400	rBV	196	154	0.01%	0.001%
28	5.643	1401	1416	1438	rBV	370230	730117	28.12%	5.717%
29	5.878	1486	1489	1493	rBV2	397	371	0.01%	0.003%
30	5.913	1497	1500	1501	rBV	979	491	0.02%	0.004%
31	6.093	1541	1556	1575	rBV	244411	498407	19.20%	3.903%
32	6.306	1620	1622	1624	rBV	295	165	0.01%	0.001%
33	6.338	1630	1632	1636	rVB2	337	234	0.01%	0.002%
34	6.363	1636	1640	1644	rBV2	239	227	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015027.D
 Acq On : 18 Mar 2020 20:48
 Operator : SY/MD
 Sample : L1941-06DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

35	6.463	1669	1671	1672	rBV2	239	54	0.00%	0.000%
36	6.486	1675	1678	1681	rBV	169	118	0.00%	0.001%
37	6.643	1725	1727	1728	rBV	269	120	0.00%	0.001%
38	6.736	1754	1756	1759	rVB	404	178	0.01%	0.001%
39	6.833	1783	1786	1791	rBV	234	203	0.01%	0.002%
40	6.913	1809	1811	1812	rBV	214	45	0.00%	0.000%
41	7.006	1828	1840	1859	rBV	141829	254805	9.82%	1.995%
42	7.161	1885	1888	1891	rVB3	521	325	0.01%	0.003%
43	7.183	1893	1895	1898	rVB	476	262	0.01%	0.002%
44	7.206	1900	1902	1906	rVB2	450	285	0.01%	0.002%
45	7.228	1906	1909	1911	rBV	263	165	0.01%	0.001%
46	7.338	1929	1943	1963	rBV	595632	1016100	39.14%	7.957%
47	7.640	2027	2037	2059	rBV2	98627	168570	6.49%	1.320%
48	7.904	2118	2119	2122	rVB2	331	139	0.01%	0.001%
49	7.923	2123	2125	2128	rVV	261	157	0.01%	0.001%
50	7.952	2132	2134	2141	rVB2	460	444	0.02%	0.003%
51	8.000	2146	2149	2154	rVB2	513	367	0.01%	0.003%
52	8.064	2166	2169	2172	rBV	346	151	0.01%	0.001%
53	8.119	2174	2186	2220	rBV	261398	573238	22.08%	4.489%
54	8.691	2362	2364	2365	rBV	274	95	0.00%	0.001%
55	8.871	2407	2420	2454	rBV2	566906	1192253	45.93%	9.336%
56	9.141	2501	2504	2505	rBV	320	154	0.01%	0.001%
57	9.273	2543	2545	2550	rVB	363	168	0.01%	0.001%
58	10.235	2832	2844	2868	rBV	369669	584065	22.50%	4.574%
59	10.341	2874	2877	2879	rBV	426	171	0.01%	0.001%
60	10.424	2900	2903	2907	rBV2	428	360	0.01%	0.003%
61	10.556	2940	2944	2950	rBV2	527	669	0.03%	0.005%
62	10.672	2977	2980	2985	rBV	354	305	0.01%	0.002%
63	10.698	2986	2988	2993	rBV	263	173	0.01%	0.001%
64	11.202	3134	3145	3155	rBV	66769	102995	3.97%	0.807%
65	11.270	3155	3166	3191	rVB2	631816	1537617	59.23%	12.040%
66	11.469	3227	3228	3230	rVB2	251	74	0.00%	0.001%
67	11.588	3260	3265	3268	rBV	429	432	0.02%	0.003%
68	11.659	3270	3287	3306	rBV2	1194446	2596054	100.00%	20.328%
69	11.871	3351	3353	3356	rBV2	290	172	0.01%	0.001%
70	11.932	3369	3372	3374	rBV2	525	322	0.01%	0.003%
71	12.009	3395	3396	3398	rBV2	310	148	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015027.D
Acq On : 18 Mar 2020 20:48
Operator : SY/MD
Sample : L1941-06DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB6DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Title : VOC Analysis

72	12.415	3520	3522	3525	rBV2	566	393	0.02%	0.003%
73	12.665	3596	3600	3612	rVB5	1647	2013	0.08%	0.016%
74	12.955	3687	3690	3692	rBV	418	264	0.01%	0.002%
75	13.283	3780	3792	3810	rBV	593428	926580	35.69%	7.256%
76	13.765	3931	3942	3963	rVB	84859	132458	5.10%	1.037%
77	14.816	4264	4269	4271	rBV4	4798	4445	0.17%	0.035%
78	15.418	4448	4456	4471	rVB2	49511	76771	2.96%	0.601%


Sum of corrected areas: 12770527

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015027.D
Acq On : 18 Mar 2020 20:48
Operator : SY/MD
Sample : L1941-06DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

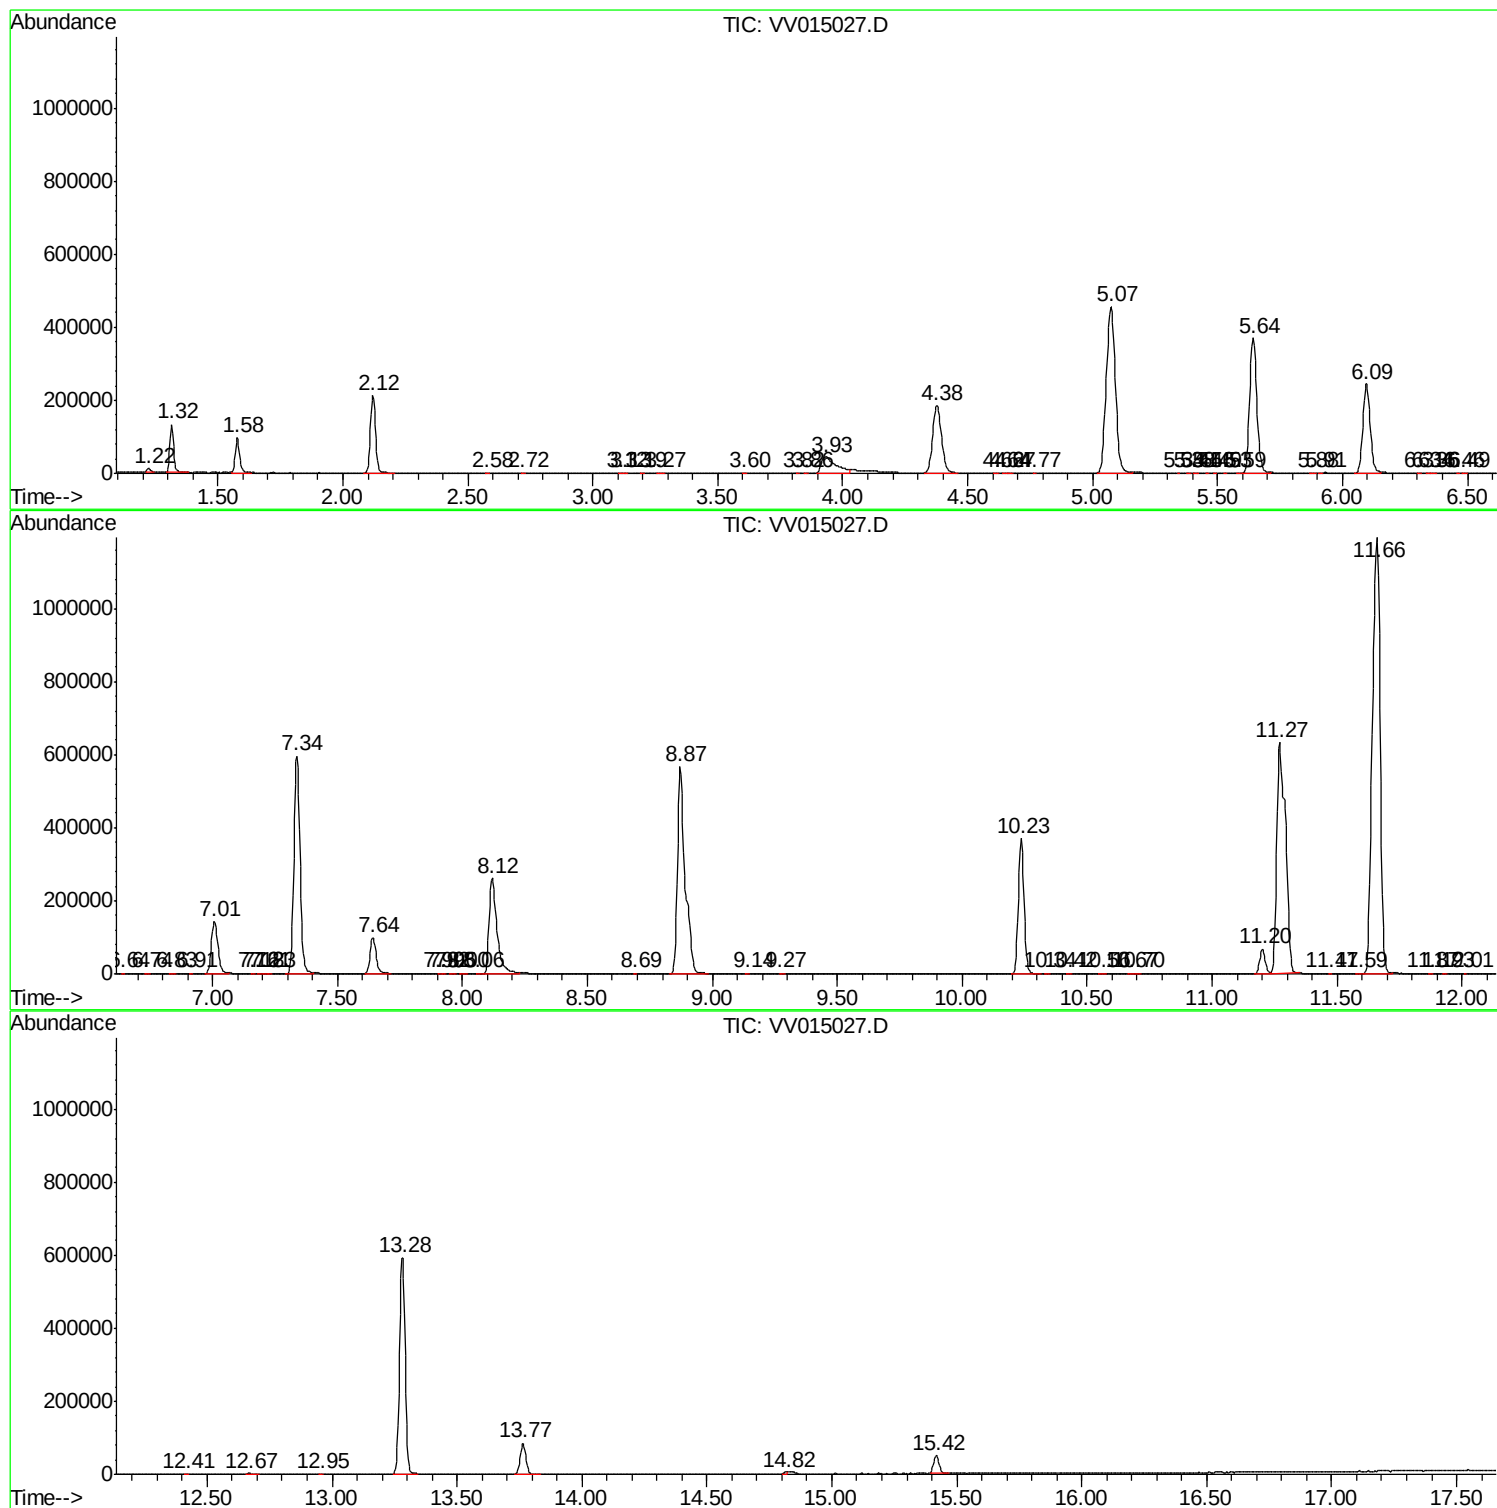

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015027.D
Acq On : 18 Mar 2020 20:48
Operator : SY/MD
Sample : L1941-06DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031820\
Data File : VV015027.D
Acq On : 18 Mar 2020 20:48
Operator : SY/MD
Sample : L1941-06DL 100X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DB6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc