

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015033.D
 Acq On : 18 Mar 2020 23:14
 Operator : SY/MD
 Sample : L1941-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	87	rVB	120852	130246	0.26%	0.143%
2	1.579	145	152	168	rVB	92353	114580	0.23%	0.126%
3	1.698	187	189	193	rBV2	933	668	0.00%	0.001%
4	2.045	296	297	300	rBV	418	227	0.00%	0.000%
5	2.122	310	321	338	rBV	201384	291283	0.58%	0.321%
6	2.865	549	552	561	rVB3	584	651	0.00%	0.001%
7	2.907	561	565	566	rBV2	318	183	0.00%	0.000%
8	2.933	571	573	574	rBV	169	51	0.00%	0.000%
9	2.971	584	585	586	rBV	153	46	0.00%	0.000%
10	3.000	592	594	597	rBV	228	79	0.00%	0.000%
11	3.248	669	671	672	rBV2	272	88	0.00%	0.000%
12	3.309	688	690	698	rVB2	305	372	0.00%	0.000%
13	3.341	698	700	702	rBV	144	72	0.00%	0.000%
14	3.611	782	784	786	rBV2	169	107	0.00%	0.000%
15	3.630	786	790	795	rVV2	351	329	0.00%	0.000%
16	3.679	802	805	807	rBV	182	107	0.00%	0.000%
17	3.737	822	823	824	rVB	264	51	0.00%	0.000%
18	3.749	824	827	829	rBV	139	95	0.00%	0.000%
19	3.833	850	853	854	rBV	169	93	0.00%	0.000%
20	3.868	861	864	867	rBV	207	148	0.00%	0.000%
21	3.929	872	883	905	rBV	42282	151289	0.30%	0.167%
22	4.380	1007	1023	1055	rVB	181205	448654	0.89%	0.494%
23	4.614	1093	1096	1099	rVB3	522	290	0.00%	0.000%
24	4.634	1099	1102	1107	rVB2	346	289	0.00%	0.000%
25	4.672	1107	1114	1118	rBV3	397	565	0.00%	0.001%
26	4.804	1153	1155	1156	rBV	260	110	0.00%	0.000%
27	4.981	1207	1210	1215	rVB2	228	161	0.00%	0.000%
28	5.007	1215	1218	1220	rBV	242	190	0.00%	0.000%
29	5.074	1221	1239	1271	rBV2	441884	1116827	2.22%	1.230%
30	5.270	1297	1300	1304	rBV2	562	385	0.00%	0.000%
31	5.354	1324	1326	1331	rVB2	328	168	0.00%	0.000%
32	5.399	1338	1340	1343	rVB2	276	124	0.00%	0.000%
33	5.421	1343	1347	1350	rVB3	511	383	0.00%	0.000%
34	5.444	1350	1354	1355	rBV2	441	304	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015033.D
 Acq On : 18 Mar 2020 23:14
 Operator : SY/MD
 Sample : L1941-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

35	5.482	1364	1366	1369	rBV2	268	162	0.00%	0.000%
36	5.643	1400	1416	1435	rBV	369682	720757	1.43%	0.794%
37	5.981	1519	1521	1522	rBV	200	64	0.00%	0.000%
38	6.097	1542	1557	1574	rBV	238725	490147	0.97%	0.540%
39	6.312	1622	1624	1625	rBV	200	60	0.00%	0.000%
40	6.344	1632	1634	1638	rBV	277	181	0.00%	0.000%
41	6.810	1775	1779	1781	rBV	399	329	0.00%	0.000%
42	6.839	1786	1788	1789	rBV	251	100	0.00%	0.000%
43	6.878	1798	1800	1801	rBV	171	49	0.00%	0.000%
44	7.007	1826	1840	1856	rBV	139759	247877	0.49%	0.273%
45	7.338	1929	1943	1964	rBV	576863	1001128	1.99%	1.103%
46	7.566	2012	2014	2017	rBV2	276	139	0.00%	0.000%
47	7.640	2027	2037	2060	rBV	98508	168334	0.33%	0.185%
48	7.820	2089	2093	2096	rBV2	380	413	0.00%	0.000%
49	7.958	2129	2136	2141	rBV3	1321	1670	0.00%	0.002%
50	7.997	2146	2148	2155	rVB4	523	466	0.00%	0.001%
51	8.119	2174	2186	2220	rBV2	241300	550055	1.09%	0.606%
52	8.447	2284	2288	2290	rVB2	322	157	0.00%	0.000%
53	8.463	2290	2293	2295	rBV	435	215	0.00%	0.000%
54	8.904	2408	2430	2472	rBV	8594996	14630884	29.02%	16.115%
55	9.244	2533	2536	2539	rBV	672	437	0.00%	0.000%
56	9.453	2598	2601	2604	rBV2	322	238	0.00%	0.000%
57	9.537	2625	2627	2630	rVB	361	163	0.00%	0.000%
58	9.637	2656	2658	2660	rBV2	190	59	0.00%	0.000%
59	9.662	2664	2666	2668	rBV2	325	132	0.00%	0.000%
60	9.907	2740	2742	2744	rBV	212	122	0.00%	0.000%
61	9.942	2751	2753	2755	rBV2	287	127	0.00%	0.000%
62	10.109	2802	2805	2806	rBV	244	124	0.00%	0.000%
63	10.235	2831	2844	2865	rBV	366931	579707	1.15%	0.639%
64	10.450	2904	2911	2913	rBV3	912	1033	0.00%	0.001%
65	10.563	2943	2946	2950	rVB2	572	459	0.00%	0.001%
66	10.666	2976	2978	2981	rVB	222	72	0.00%	0.000%
67	10.707	2987	2991	2994	rBV2	233	223	0.00%	0.000%
68	10.871	3040	3042	3045	rBV2	411	199	0.00%	0.000%
69	10.939	3058	3063	3065	rBV2	609	507	0.00%	0.001%
70	11.048	3096	3097	3098	rBV	226	60	0.00%	0.000%
71	11.100	3110	3113	3118	rBV2	371	358	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015033.D
 Acq On : 18 Mar 2020 23:14
 Operator : SY/MD
 Sample : L1941-12
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

72	11.199	3132	3144	3156	rBV	951500	1458976	2.89%	1.607%
73	11.293	3156	3173	3199	rVB2	3524566	6237675	12.37%	6.871%
74	11.550	3249	3253	3257	rBV4	1184	1257	0.00%	0.001%
75	11.672	3271	3291	3309	rBV	30080307	50414752	100.00%	55.530%
76	12.312	3487	3490	3492	rBV	492	400	0.00%	0.000%
77	12.415	3513	3522	3538	rVB	48384	72205	0.14%	0.080%
78	12.608	3569	3582	3591	rBV6	7244	17042	0.03%	0.019%
79	12.669	3594	3601	3608	rVB3	5108	6850	0.01%	0.008%
80	12.768	3623	3632	3642	rBV2	18583	28729	0.06%	0.032%
81	13.283	3778	3792	3812	rBV	6738477	10091426	20.02%	11.115%
82	13.762	3929	3941	3961	rBV	1089421	1668951	3.31%	1.838%
83	14.839	4264	4276	4289	rVB	48914	83532	0.17%	0.092%
84	15.418	4449	4456	4471	rVB3	32443	50201	0.10%	0.055%


Sum of corrected areas: 90788418

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015033.D
Acq On : 18 Mar 2020 23:14
Operator : SY/MD
Sample : L1941-12
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

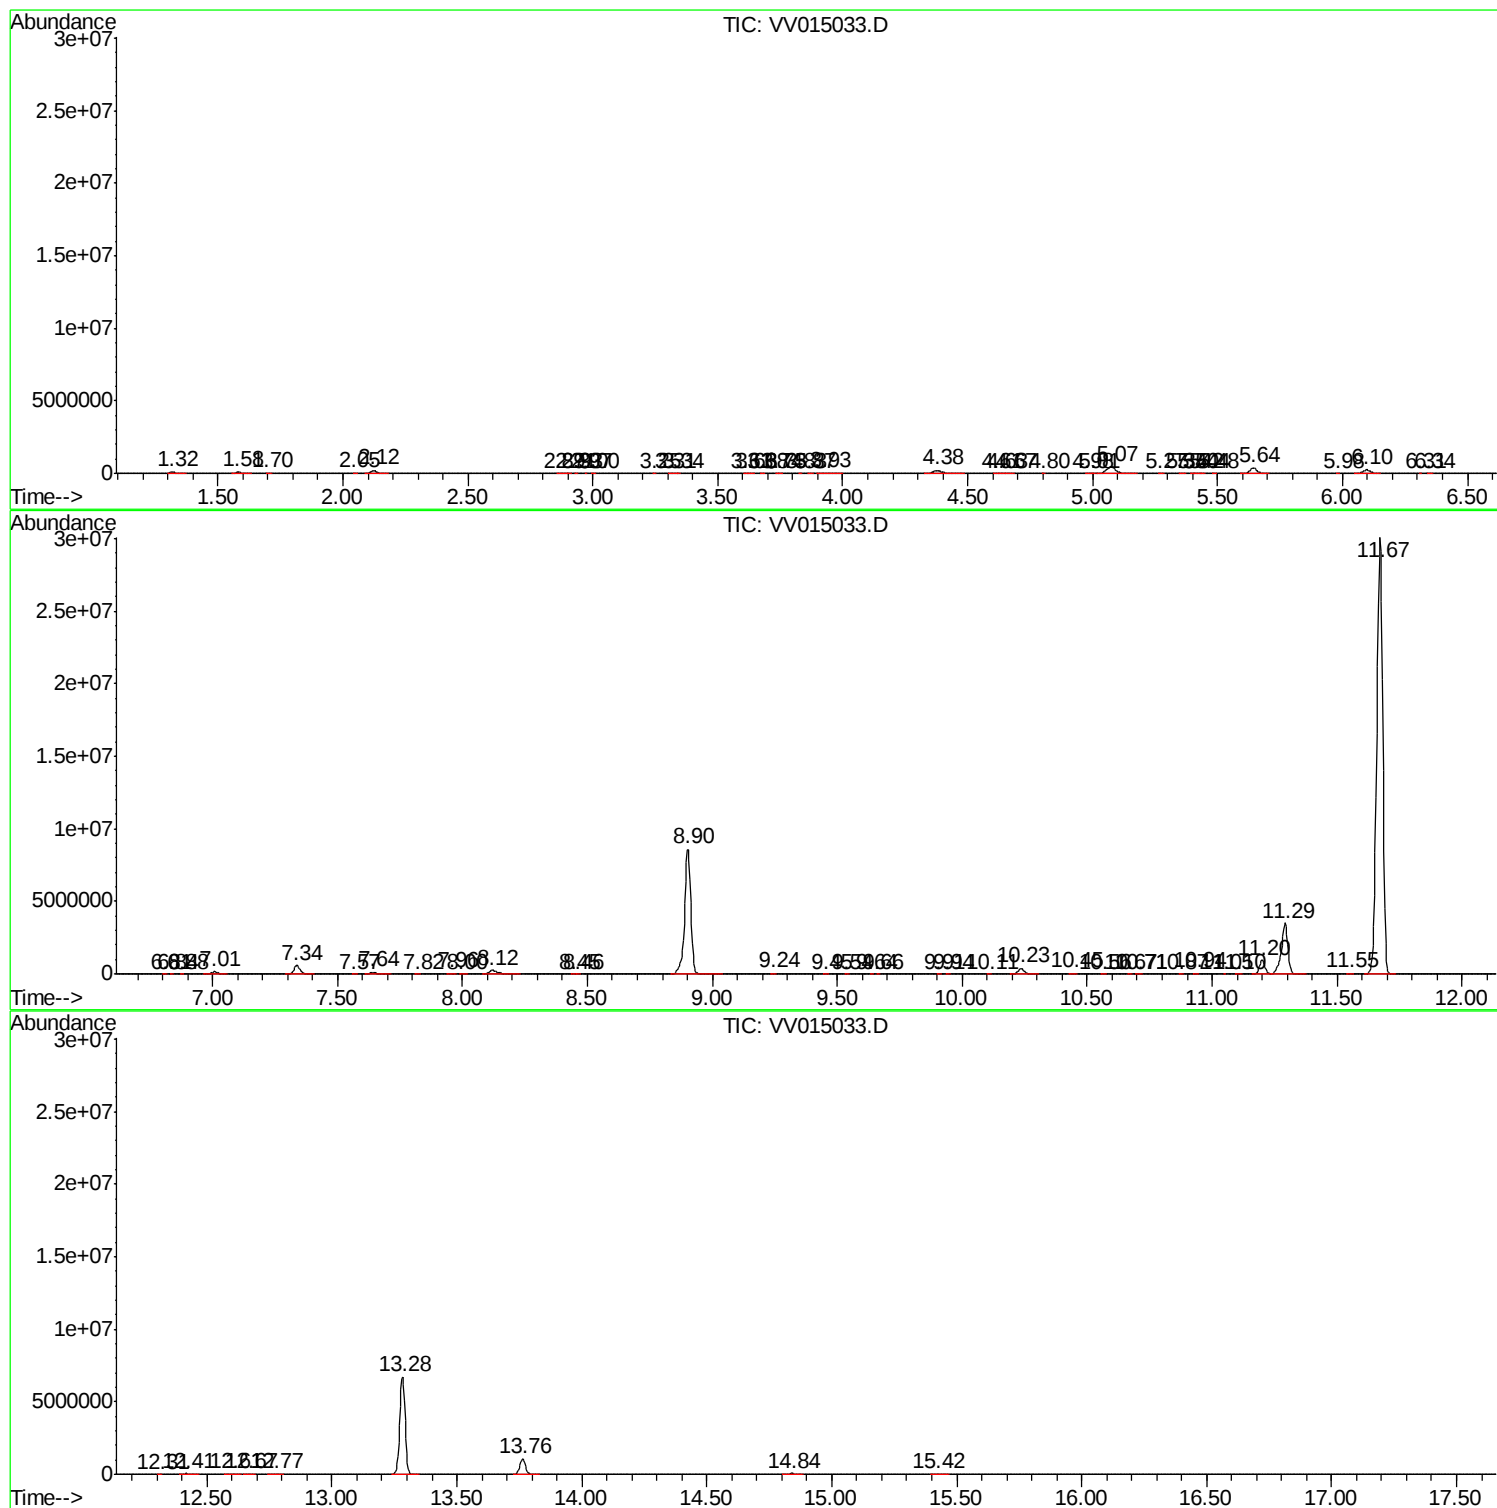

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015033.D
Acq On : 18 Mar 2020 23:14
Operator : SY/MD
Sample : L1941-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015033.D
Acq On : 18 Mar 2020 23:14
Operator : SY/MD
Sample : L1941-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc