

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015036.D
 Acq On : 19 Mar 2020 00:27
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	88	rVB	125715	134024	8.95%	1.232%
2	1.579	145	152	167	rVB	99012	118629	7.93%	1.091%
3	2.061	300	302	303	rBV	564	229	0.02%	0.002%
4	2.122	309	321	338	rBV	204250	298119	19.92%	2.741%
5	2.846	543	546	551	rVB2	320	315	0.02%	0.003%
6	2.878	551	556	557	rBV2	465	410	0.03%	0.004%
7	2.978	585	587	589	rBV	188	76	0.01%	0.001%
8	3.026	600	602	609	rVB	349	253	0.02%	0.002%
9	3.093	621	623	624	rVB	136	35	0.00%	0.000%
10	3.110	624	628	632	rBV2	335	200	0.01%	0.002%
11	3.437	726	730	733	rBV	337	283	0.02%	0.003%
12	3.508	749	752	754	rBV	122	78	0.01%	0.001%
13	3.569	769	771	774	rVB2	289	179	0.01%	0.002%
14	3.589	774	777	778	rBV	257	172	0.01%	0.002%
15	3.653	794	797	799	rBV	232	182	0.01%	0.002%
16	3.704	810	813	816	rBV2	387	245	0.02%	0.002%
17	3.817	844	848	849	rBV	127	95	0.01%	0.001%
18	3.849	853	858	860	rBV	309	267	0.02%	0.002%
19	3.936	872	885	918	rBV2	41678	176878	11.82%	1.626%
20	4.380	1005	1023	1050	rVB2	184892	456861	30.52%	4.200%
21	4.601	1089	1092	1095	rBV2	229	138	0.01%	0.001%
22	4.756	1136	1140	1142	rBV	311	216	0.01%	0.002%
23	4.814	1156	1158	1163	rBV2	256	159	0.01%	0.001%
24	4.878	1177	1178	1181	rBV	232	159	0.01%	0.001%
25	5.074	1220	1239	1273	rBV2	453653	1222452	81.67%	11.238%
26	5.408	1340	1343	1346	rBV2	342	229	0.02%	0.002%
27	5.425	1346	1348	1350	rBV	292	151	0.01%	0.001%
28	5.537	1381	1383	1385	rVB2	309	127	0.01%	0.001%
29	5.643	1402	1416	1438	rBV	358179	714968	47.77%	6.573%
30	5.926	1497	1504	1507	rBV6	1613	2139	0.14%	0.020%
31	5.971	1516	1518	1523	rVB2	402	302	0.02%	0.003%
32	6.000	1525	1527	1530	rBV2	320	135	0.01%	0.001%
33	6.016	1530	1532	1534	rBV	273	142	0.01%	0.001%
34	6.097	1541	1557	1581	rBV	247403	497524	33.24%	4.574%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015036.D
 Acq On : 19 Mar 2020 00:27
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

35	6.338	1629	1632	1635	rVB2	366	214	0.01%	0.002%
36	6.357	1635	1638	1644	rBV2	323	249	0.02%	0.002%
37	6.415	1653	1656	1658	rBV	175	122	0.01%	0.001%
38	6.450	1661	1667	1671	rBV	246	256	0.02%	0.002%
39	6.531	1691	1692	1693	rBV	250	50	0.00%	0.000%
40	6.550	1696	1698	1701	rBV2	305	202	0.01%	0.002%
41	6.775	1766	1768	1769	rBV	249	104	0.01%	0.001%
42	6.807	1777	1778	1784	rVB	252	146	0.01%	0.001%
43	6.904	1806	1808	1811	rVB2	178	75	0.01%	0.001%
44	6.926	1811	1815	1818	rBV2	340	271	0.02%	0.002%
45	7.006	1829	1840	1861	rBV	139834	248892	16.63%	2.288%
46	7.132	1876	1879	1882	rBV	336	199	0.01%	0.002%
47	7.170	1887	1891	1892	rBV2	563	361	0.02%	0.003%
48	7.206	1900	1902	1904	rBV	437	238	0.02%	0.002%
49	7.338	1927	1943	1979	rBV	576219	1007970	67.34%	9.266%
50	7.643	2027	2038	2055	rBV2	95192	165714	11.07%	1.523%
51	7.772	2075	2078	2080	rBV	428	267	0.02%	0.002%
52	7.794	2083	2085	2087	rVV	210	71	0.00%	0.001%
53	7.817	2090	2092	2094	rVB2	303	144	0.01%	0.001%
54	7.859	2103	2105	2106	rBV	209	86	0.01%	0.001%
55	7.894	2113	2116	2118	rBV	233	163	0.01%	0.001%
56	8.003	2147	2150	2154	rVB	465	277	0.02%	0.003%
57	8.029	2154	2158	2160	rBV2	325	222	0.01%	0.002%
58	8.122	2175	2187	2240	rBV2	240078	554323	37.03%	5.096%
59	8.531	2310	2314	2316	rBV2	338	284	0.02%	0.003%
60	8.871	2408	2420	2427	rBV	553505	992971	66.34%	9.128%
61	9.103	2491	2492	2496	rVB2	314	137	0.01%	0.001%
62	9.164	2506	2511	2518	rBV3	876	914	0.06%	0.008%
63	9.325	2559	2561	2562	rBV	162	47	0.00%	0.000%
64	9.604	2645	2648	2649	rBV2	217	113	0.01%	0.001%
65	9.640	2658	2659	2660	rBV2	164	53	0.00%	0.000%
66	9.685	2672	2673	2674	rVB2	173	33	0.00%	0.000%
67	9.765	2696	2698	2702	rBV2	208	142	0.01%	0.001%
68	9.920	2744	2746	2748	rBV	287	95	0.01%	0.001%
69	9.974	2761	2763	2766	rVB2	259	112	0.01%	0.001%
70	10.235	2833	2844	2867	rBV	366606	577058	38.55%	5.305%
71	10.408	2890	2898	2901	rBV2	699	955	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015036.D
 Acq On : 19 Mar 2020 00:27
 Operator : SY/MD
 Sample : L1941-18
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DL8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

72	10.501	2924	2927	2929	rBV	308	179	0.01%	0.002%
73	10.592	2951	2955	2956	rBV	257	133	0.01%	0.001%
74	10.669	2976	2979	2981	rBV2	285	189	0.01%	0.002%
75	10.936	3057	3062	3065	rVB2	664	577	0.04%	0.005%
76	11.202	3134	3145	3155	rBV2	54976	88223	5.89%	0.811%
77	11.270	3155	3166	3191	rVB2	610754	1388208	92.75%	12.762%
78	11.553	3252	3254	3258	rBV	317	195	0.01%	0.002%
79	11.575	3258	3261	3264	rBV3	543	443	0.03%	0.004%
80	11.646	3269	3283	3306	rBV3	698282	1496763	100.00%	13.760%
81	12.418	3516	3523	3532	rBV6	4337	6631	0.44%	0.061%
82	12.588	3573	3576	3577	rBV	1080	559	0.04%	0.005%
83	12.665	3594	3600	3609	rVB5	2717	3889	0.26%	0.036%
84	12.768	3626	3632	3641	rBV4	3121	4185	0.28%	0.038%
85	12.826	3647	3650	3654	rBV2	493	276	0.02%	0.003%
86	13.280	3780	3791	3806	rBV	338179	523551	34.98%	4.813%
87	13.765	3930	3942	3954	rBV2	108192	170970	11.42%	1.572%
88	15.418	4450	4456	4467	rBV4	8844	12836	0.86%	0.118%


Sum of corrected areas: 10877708

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015036.D
Acq On : 19 Mar 2020 00:27
Operator : SY/MD
Sample : L1941-18
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

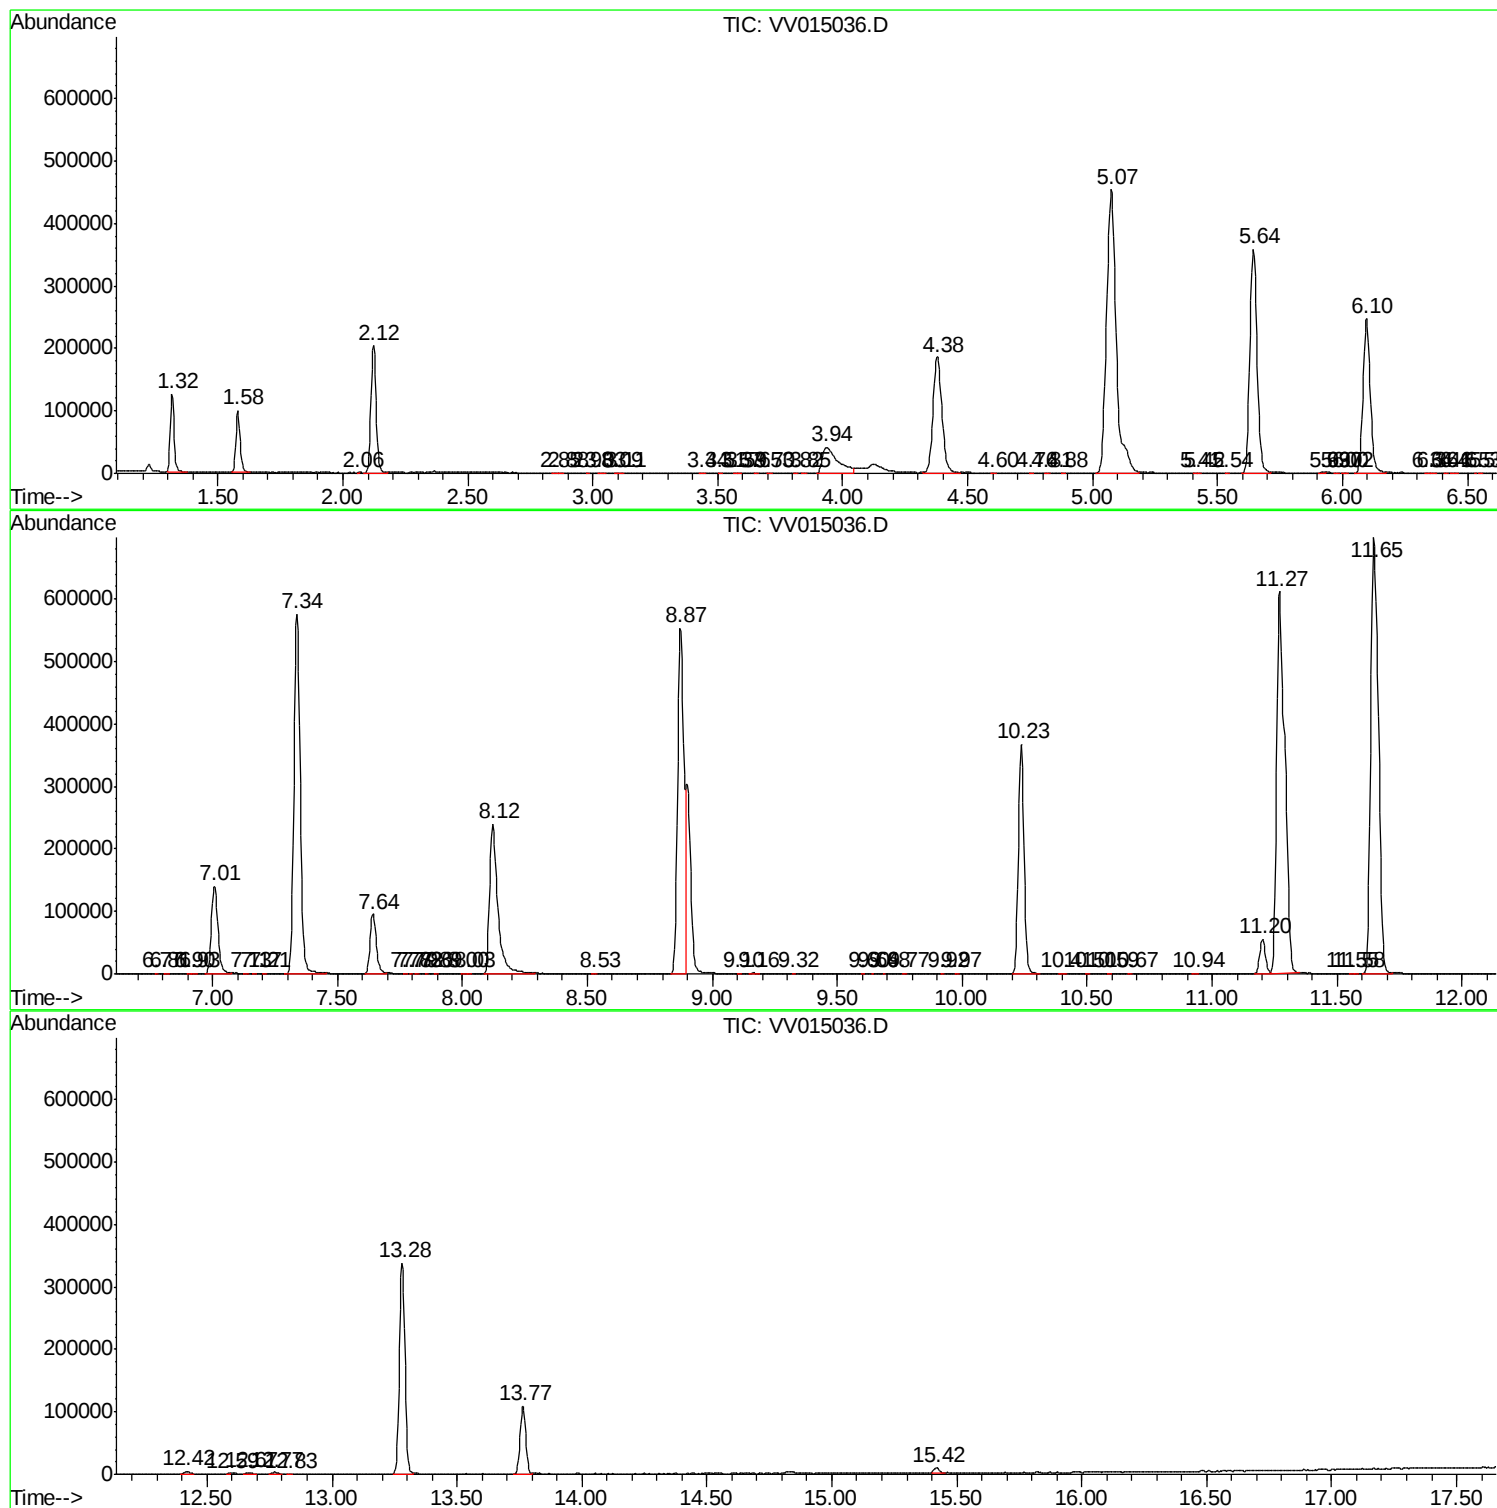

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015036.D
Acq On : 19 Mar 2020 00:27
Operator : SY/MD
Sample : L1941-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015036.D
Acq On : 19 Mar 2020 00:27
Operator : SY/MD
Sample : L1941-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DL8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc