

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015041.D
 Acq On : 19 Mar 2020 02:28
 Operator : SY/MD
 Sample : L1941-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DM0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.222	36	41	48	rBV2	12729	12658	0.01%	0.003%
2	1.315	63	70	90	rVB	170728	185229	0.13%	0.040%
3	1.579	144	152	169	rVB	101864	121649	0.08%	0.026%
4	1.765	208	210	219	rVB8	1641	1789	0.00%	0.000%
5	2.010	279	286	290	rBV5	1443	1853	0.00%	0.000%
6	2.122	310	321	338	rVV	211578	307044	0.21%	0.066%
7	2.193	338	343	348	rBV7	1408	1760	0.00%	0.000%
8	2.293	371	374	376	rBV3	820	633	0.00%	0.000%
9	2.351	386	392	394	rBV4	1252	1365	0.00%	0.000%
10	2.788	517	528	532	rBV5	1971	3034	0.00%	0.001%
11	3.061	609	613	615	rVV2	429	366	0.00%	0.000%
12	3.457	732	736	739	rBV3	634	414	0.00%	0.000%
13	3.524	753	757	761	rBV2	293	293	0.00%	0.000%
14	3.791	826	840	855	rBV4	12772	32304	0.02%	0.007%
15	3.929	868	883	917	rBV2	45034	185924	0.13%	0.040%
16	4.379	1005	1023	1052	rBV3	204359	588477	0.40%	0.127%
17	4.592	1085	1089	1092	rBV3	512	304	0.00%	0.000%
18	4.707	1110	1125	1141	rVB4	8157	20643	0.01%	0.004%
19	4.791	1145	1151	1155	rBV3	587	685	0.00%	0.000%
20	4.859	1155	1172	1193	rVB2	55208	135043	0.09%	0.029%
21	4.942	1193	1198	1202	rVB2	574	501	0.00%	0.000%
22	5.132	1220	1257	1312	rBV	13782661	31596980	21.54%	6.836%
23	5.505	1370	1373	1378	rVB5	883	699	0.00%	0.000%
24	5.643	1403	1416	1439	rBV	391811	770511	0.53%	0.167%
25	5.781	1456	1459	1467	rVB3	449	499	0.00%	0.000%
26	5.939	1498	1508	1516	rVB10	2458	4584	0.00%	0.001%
27	6.026	1532	1535	1542	rVB4	392	359	0.00%	0.000%
28	6.096	1542	1557	1591	rBV2	248747	535333	0.36%	0.116%
29	6.228	1591	1598	1599	rBV4	875	761	0.00%	0.000%
30	6.389	1638	1648	1655	rVV7	1786	2377	0.00%	0.001%
31	6.646	1723	1728	1730	rBV2	702	633	0.00%	0.000%
32	6.704	1744	1746	1750	rBV3	515	361	0.00%	0.000%
33	6.820	1775	1782	1788	rVB5	794	892	0.00%	0.000%
34	7.006	1828	1840	1865	rVV	148615	267157	0.18%	0.058%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015041.D
 Acq On : 19 Mar 2020 02:28
 Operator : SY/MD
 Sample : L1941-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DM0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

35	7.161	1884	1888	1891	rBV3	570	380	0.00%	0.000%
36	7.190	1893	1897	1902	rVB3	395	353	0.00%	0.000%
37	7.338	1928	1943	1960	rBV	611084	1064128	0.73%	0.230%
38	7.588	2014	2021	2023	rBV2	248	311	0.00%	0.000%
39	7.640	2023	2037	2056	rBV	106035	180536	0.12%	0.039%
40	7.727	2062	2064	2067	rVB2	505	286	0.00%	0.000%
41	7.955	2130	2135	2138	rBV3	783	535	0.00%	0.000%
42	7.997	2139	2148	2158	rVB3	7246	11721	0.01%	0.003%
43	8.067	2165	2170	2174	rBV2	322	388	0.00%	0.000%
44	8.119	2174	2186	2219	rBV	257790	561181	0.38%	0.121%
45	8.379	2264	2267	2271	rVB2	439	285	0.00%	0.000%
46	8.759	2382	2385	2390	rBV2	375	427	0.00%	0.000%
47	8.916	2407	2434	2479	rBV2	41356180	79746043	54.37%	17.254%
48	9.463	2599	2604	2608	rBV4	675	710	0.00%	0.000%
49	9.755	2693	2695	2699	rBV3	761	499	0.00%	0.000%
50	9.862	2725	2728	2730	rVV2	476	294	0.00%	0.000%
51	9.897	2737	2739	2744	rBV3	418	331	0.00%	0.000%
52	9.958	2752	2758	2761	rVB3	611	542	0.00%	0.000%
53	9.974	2761	2763	2766	rVB2	603	336	0.00%	0.000%
54	10.000	2766	2771	2775	rBV	382	423	0.00%	0.000%
55	10.042	2781	2784	2791	rBV3	442	387	0.00%	0.000%
56	10.109	2801	2805	2807	rBV4	474	342	0.00%	0.000%
57	10.190	2824	2830	2832	rBV2	659	719	0.00%	0.000%
58	10.238	2832	2845	2867	rVB2	443354	703180	0.48%	0.152%
59	10.408	2895	2898	2900	rVV2	451	342	0.00%	0.000%
60	10.444	2901	2909	2922	rVB2	22289	34401	0.02%	0.007%
61	10.559	2936	2945	2957	rVB3	10578	15741	0.01%	0.003%
62	10.739	2996	3001	3004	rBV2	264	290	0.00%	0.000%
63	10.874	3037	3043	3045	rBV2	496	449	0.00%	0.000%
64	10.935	3058	3062	3065	rVV3	756	692	0.00%	0.000%
65	10.961	3068	3070	3073	rVV2	507	319	0.00%	0.000%
66	11.029	3085	3091	3096	rBV3	312	374	0.00%	0.000%
67	11.080	3104	3107	3113	rBV4	1090	995	0.00%	0.000%
68	11.206	3126	3146	3159	rBV	16374348	26107136	17.80%	5.648%
69	11.312	3159	3179	3199	rVB3	57699031	110807791	75.54%	23.974%
70	11.691	3272	3297	3312	rBV3	68496931	146683839	100.00%	31.736%
71	12.128	3429	3433	3442	rVB7	3376	4674	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031820\
 Data File : VV015041.D
 Acq On : 19 Mar 2020 02:28
 Operator : SY/MD
 Sample : L1941-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DM0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis

72	12.415	3512	3522	3538	rVB	165603	249863	0.17%	0.054%
73	12.595	3567	3578	3590	rBV4	42243	102264	0.07%	0.022%
74	12.659	3590	3598	3617	rVB2	75689	126482	0.09%	0.027%
75	12.768	3621	3632	3646	rVB2	104842	161546	0.11%	0.035%
76	12.865	3658	3662	3664	rBV2	762	543	0.00%	0.000%
77	13.019	3701	3710	3719	rVB4	7977	13926	0.01%	0.003%
78	13.077	3725	3728	3732	rBV5	613	608	0.00%	0.000%
79	13.119	3737	3741	3748	rBV5	1262	1612	0.00%	0.000%
80	13.148	3748	3750	3752	rBV4	651	307	0.00%	0.000%
81	13.183	3758	3761	3763	rBV2	607	358	0.00%	0.000%
82	13.202	3764	3767	3769	rBV5	652	404	0.00%	0.000%
83	13.289	3774	3794	3820	rBV	27223373	41962647	28.61%	9.079%
84	13.527	3861	3868	3880	rVB3	2973	5511	0.00%	0.001%
85	13.765	3927	3942	3971	rBV	10952239	16529603	11.27%	3.576%
86	14.022	4020	4022	4024	rBV3	635	292	0.00%	0.000%
87	14.099	4044	4046	4049	rBV2	815	340	0.00%	0.000%
88	14.167	4055	4067	4079	rBV2	15540	25693	0.02%	0.006%
89	14.225	4083	4085	4089	rVB3	896	605	0.00%	0.000%
90	14.315	4098	4113	4126	rVB6	9971	25308	0.02%	0.005%
91	14.402	4137	4140	4141	rBV2	653	388	0.00%	0.000%
92	14.492	4166	4168	4174	rVB4	1076	728	0.00%	0.000%
93	14.517	4174	4176	4178	rBV3	1547	1079	0.00%	0.000%
94	14.559	4187	4189	4193	rVB2	887	564	0.00%	0.000%
95	14.630	4205	4211	4225	rVB2	3318	5984	0.00%	0.001%
96	14.749	4244	4248	4249	rBV3	663	481	0.00%	0.000%
97	14.839	4260	4276	4293	rVB	373844	641870	0.44%	0.139%
98	15.131	4362	4367	4370	rBV5	1268	1205	0.00%	0.000%
99	15.173	4378	4380	4384	rBV4	812	564	0.00%	0.000%
100	15.414	4443	4455	4472	rBV	1046270	1626527	1.11%	0.352%


Sum of corrected areas: 462201796

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031820\
Data File : VV015041.D
Acq On : 19 Mar 2020 02:28
Operator : SY/MD
Sample : L1941-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DM0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

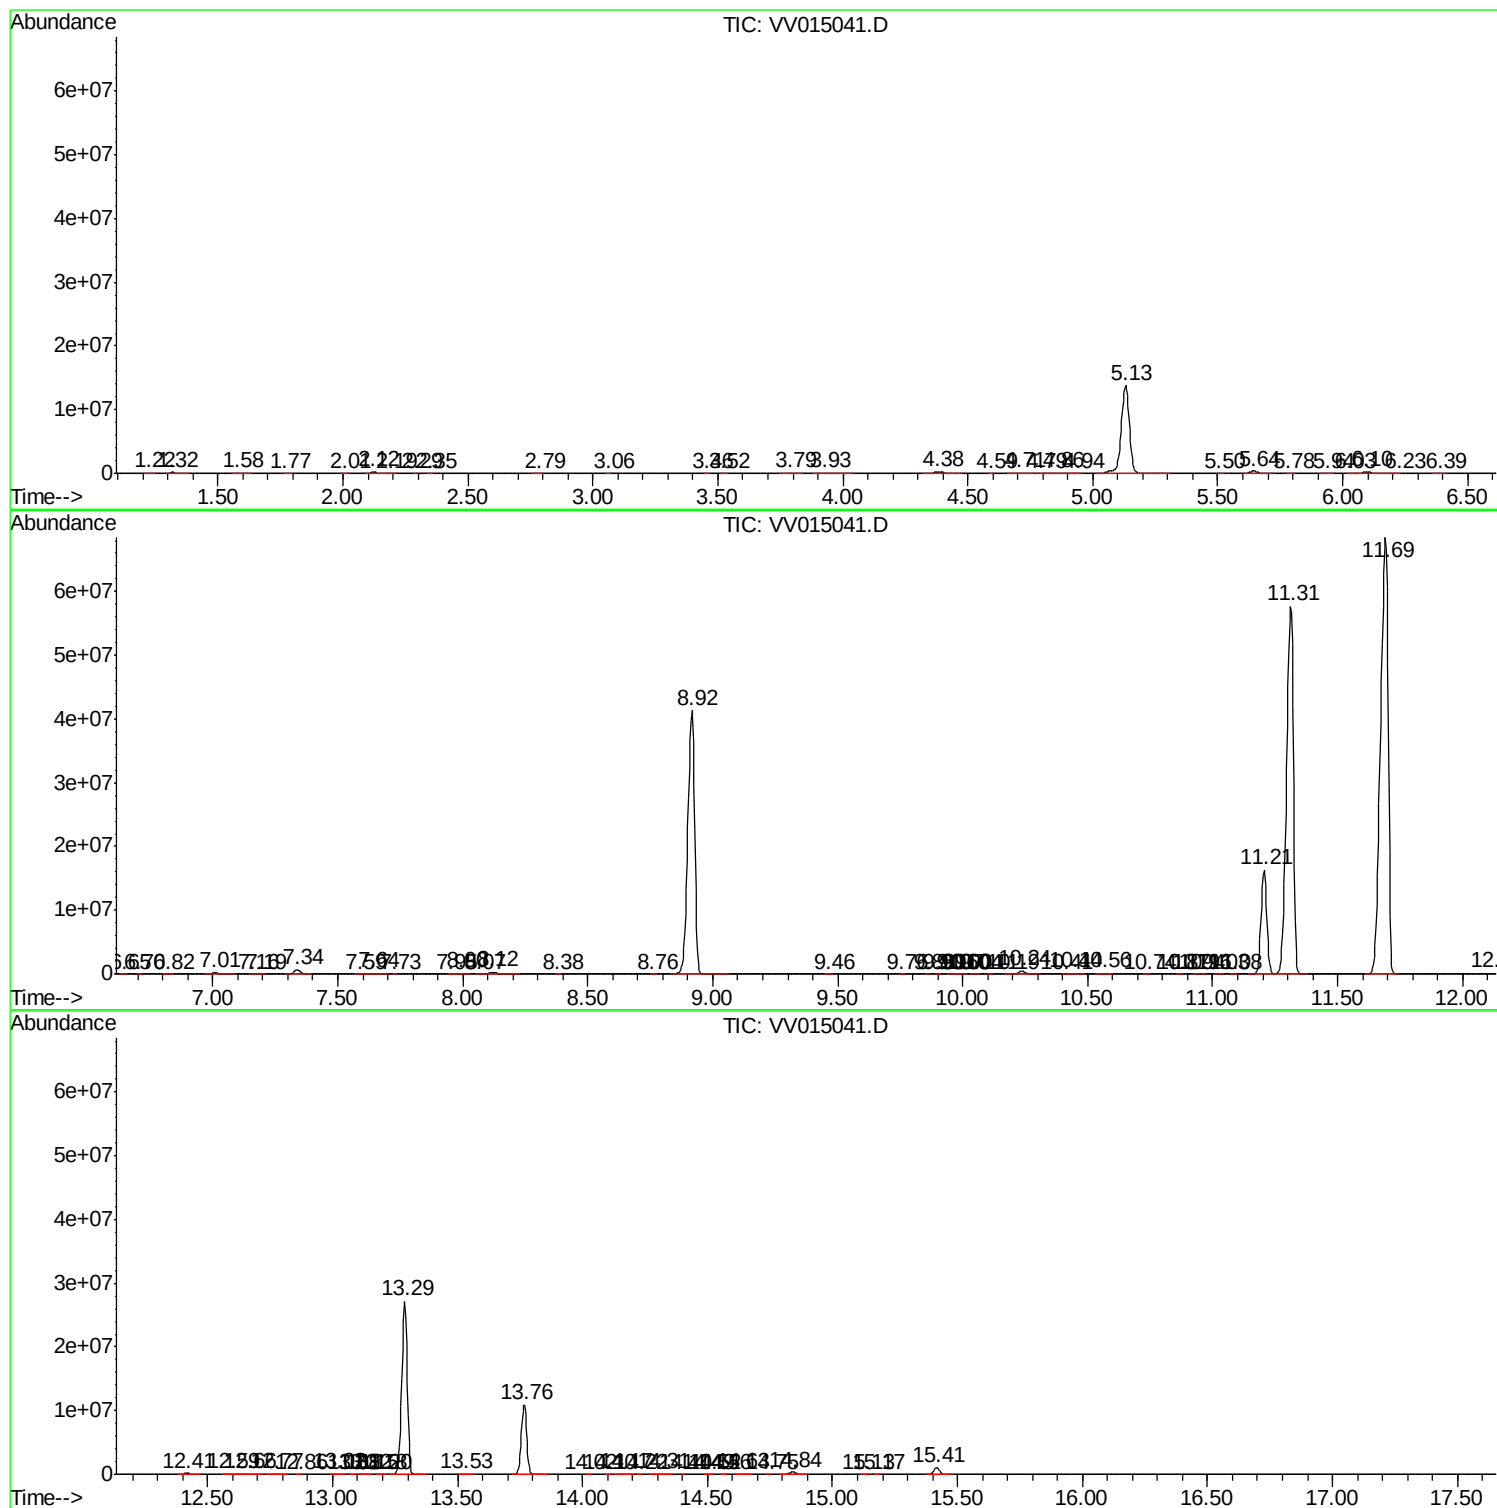

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031820\
Data File : VV015041.D
Acq On : 19 Mar 2020 02:28
Operator : SY/MD
Sample : L1941-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DM0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV031820\
Data File : VV015041.D
Acq On : 19 Mar 2020 02:28
Operator : SY/MD
Sample : L1941-20
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0DM0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM031820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
