


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031820\
 Data File : VV015013.D
 Acq On : 18 Mar 2020 09:57
 Operator : SY/MD
 Sample : BFB66
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB66

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031820WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 19 04:08:09 2020

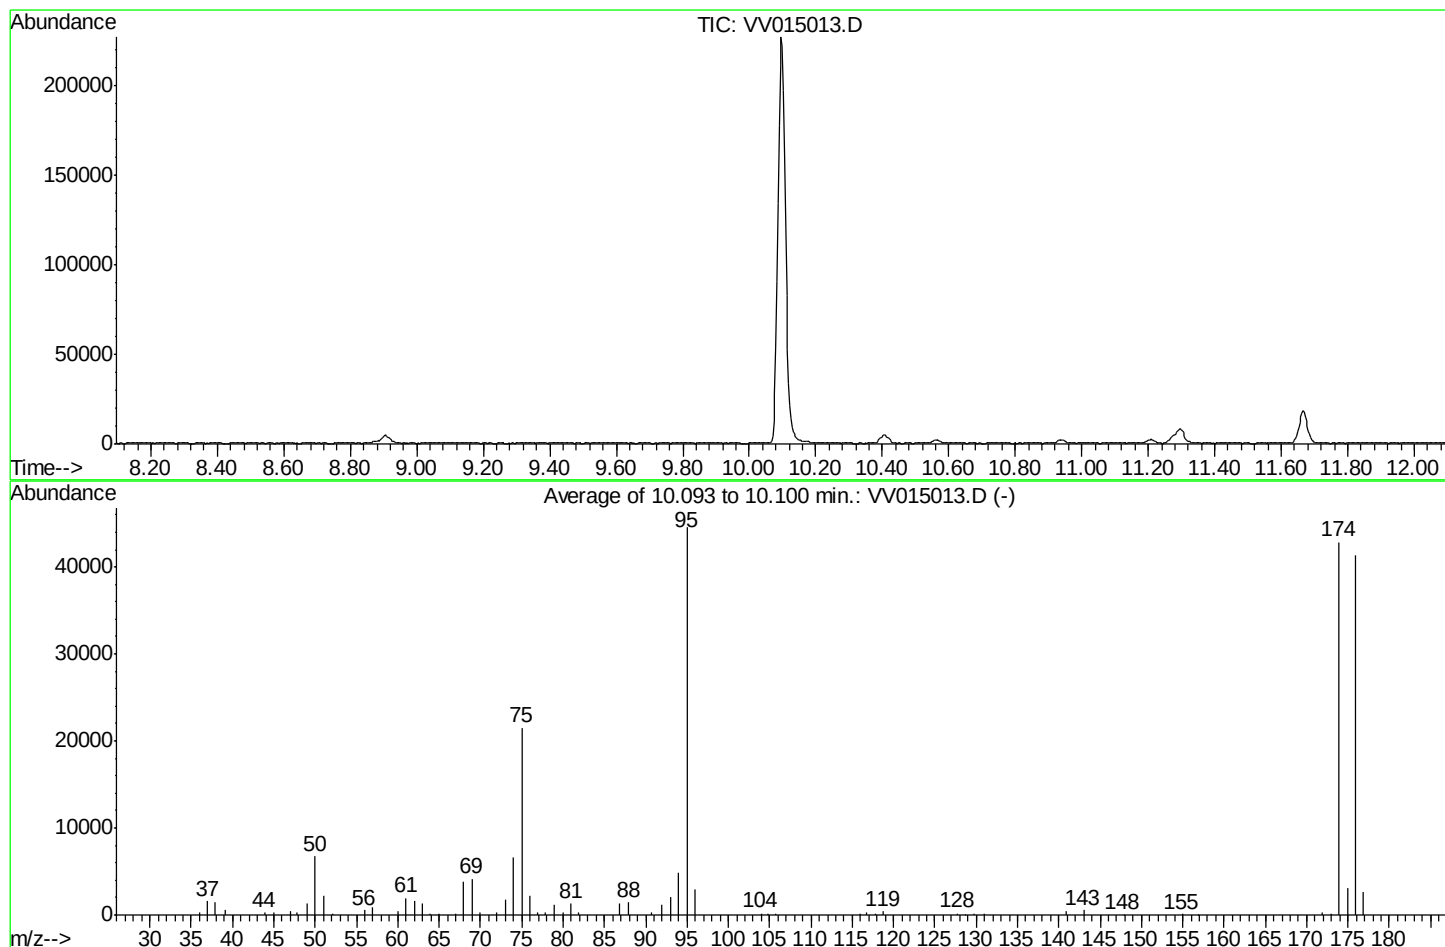

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	6716	PASS
75	95	30	80	48.2	21480	PASS
95	95	100	100	100.0	44549	PASS
96	95	5	9	6.5	2917	PASS
173	174	0.00	2	0.3	144	PASS
174	95	50	120	96.2	42853	PASS
175	174	5	9	7.3	3141	PASS
176	174	95	101	96.4	41330	PASS
177	176	5	9	6.3	2612	PASS

m/z	Abundance
35.90	286.0
37.00	1523.0
38.00	1387.0
39.10	596.0
39.90	334.0
44.00	412.0
44.90	208.0
47.10	410.0
47.80	219.0
49.00	1304.0
50.00	6637.0
51.00	2174.0
52.10	114.0
56.00	480.0
57.00	928.0
59.90	484.0
61.00	1906.0
62.10	1619.0
63.00	1249.0
63.90	221.0
65.10	194.0
67.00	149.0
68.00	3720.0
69.00	4021.0
70.00	341.0
72.10	260.0
73.00	1777.0
74.00	6581.0
75.00	21112.0
76.00	2163.0
76.90	328.0
77.90	211.0
79.00	1153.0
80.00	356.0
81.00	1273.0
81.80	286.0
86.90	1415.0
88.00	1318.0
90.70	207.0
91.90	1266.0
93.00	2228.0
94.00	4675.0
95.00	43584.0
96.00	2687.0
103.90	265.0
104.80	126.0
105.70	232.0
115.90	160.0
116.70	222.0
117.70	169.0
118.80	366.0
127.80	180.0
129.70	140.0
131.00	125.0
140.90	495.0
142.90	546.0
147.80	107.0
155.00	116.0
171.90	270.0
173.90	40168.0
174.90	3144.0
175.90	38024.0
176.90	2453.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	358.0
37.00	1552.0
37.90	1474.0
39.10	624.0
39.90	323.0
43.90	453.0
45.00	212.0
47.00	433.0
47.80	285.0
49.00	1313.0
50.00	6843.0
51.00	2209.0
52.10	124.0
56.00	578.0
57.00	940.0
60.00	466.0
61.00	2008.0
62.10	1752.0
63.00	1362.0
63.90	160.0
65.00	215.0
67.00	173.0
68.00	3871.0
69.00	4330.0
70.00	373.0
72.00	235.0
73.00	1776.0
74.00	6855.0
75.00	22144.0
76.00	2290.0
77.00	269.0
77.90	254.0
79.00	1173.0
80.00	369.0
81.00	1370.0
81.90	272.0
86.90	1385.0
87.90	1450.0
90.70	249.0
91.90	1214.0
93.00	2240.0
94.00	5055.0
95.00	45968.0
96.00	2980.0
104.00	226.0
104.80	214.0
105.80	179.0
115.90	202.0
116.70	248.0
117.70	213.0
118.80	409.0
127.80	175.0
128.70	103.0
129.70	180.0
130.90	132.0
140.90	471.0
143.00	552.0
154.90	132.0
156.90	118.0
171.90	307.0
173.90	44328.0
174.90	3255.0
175.90	42896.0
176.90	2699.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

m/z	Abundance
36.00	347.0
37.00	1579.0
37.90	1355.0
39.00	548.0
39.90	260.0
43.90	499.0
45.00	258.0
47.00	432.0
47.80	309.0
49.00	1187.0
50.00	6668.0
51.00	2057.0
52.10	137.0
56.00	579.0
57.00	846.0
60.00	394.0
61.00	1901.0
62.10	1707.0
63.00	1446.0
63.90	118.0
65.00	259.0
66.90	171.0
68.00	4021.0
69.00	4202.0
70.00	378.0
71.90	210.0
73.00	1722.0
74.00	6516.0
75.00	21184.0
76.00	2044.0
77.00	191.0
77.90	221.0
78.90	1019.0
79.90	321.0
81.00	1236.0
81.90	228.0
86.90	1286.0
87.90	1520.0
90.70	241.0
91.90	1125.0
93.00	1908.0
94.00	4788.0
95.00	44096.0
96.00	3084.0
104.00	185.0
104.80	209.0
105.90	175.0
115.90	209.0
116.80	232.0
117.80	205.0
118.80	354.0
127.70	194.0
128.70	120.0
129.80	193.0
130.90	129.0
140.80	438.0
143.10	574.0
154.90	109.0
156.90	106.0
171.90	386.0
173.00	433.0
173.90	44064.0
174.90	3025.0
175.90	43072.0
176.90	2685.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66

Scan 2789 (10.058 min): VV015013.D
BFB66

m/z	Abundance
39.90	368.0
43.80	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB66