

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031821\
 Data File : VV020666.D
 Acq On : 18 Mar 2021 10:39
 Operator : SY/MD
 Sample : VV0318MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Quant Time: Mar 19 03:59:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 19 03:58:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	441936	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	435764	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	195891	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	138073	38.73	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.46%		
7) Chloroethane-d5	1.568	69	112608	39.48	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.96%		
11) 1,1-Dichloroethene-d2	2.108	63	196221	28.96	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	57.92%#		
21) 2-Butanone-d5	3.899	46	222053	97.05	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.05%		
24) Chloroform-d	4.352	84	263802	42.57	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.14%		
26) 1,2-Dichloroethane-d4	5.034	65	182347	44.60	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.20%		
32) Benzene-d6	5.050	84	531356	44.13	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.26%		
36) 1,2-Dichloropropane-d6	6.069	67	176067	45.71	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.42%		
41) Toluene-d8	7.317	98	457804	42.78	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.56%		
43) trans-1,3-Dichloroprop...	7.622	79	76242	42.35	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.70%		
47) 2-Hexanone-d5	8.092	63	129602	89.93	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.93%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	211229	43.88	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.76%		
64) 1,2-Dichlorobenzene-d4	11.632	152	180792	47.63	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.26%		
Target Compounds					Qvalue	
48) 2-Hexanone	8.095	43	19296	4.78	ug/L #	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031821\
Data File : VV020666.D
Acq On : 18 Mar 2021 10:39
Operator : SY/MD
Sample : VV0318MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72


Quant Time: Mar 19 03:59:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 19 03:58:36 2021
Response via : Initial Calibration

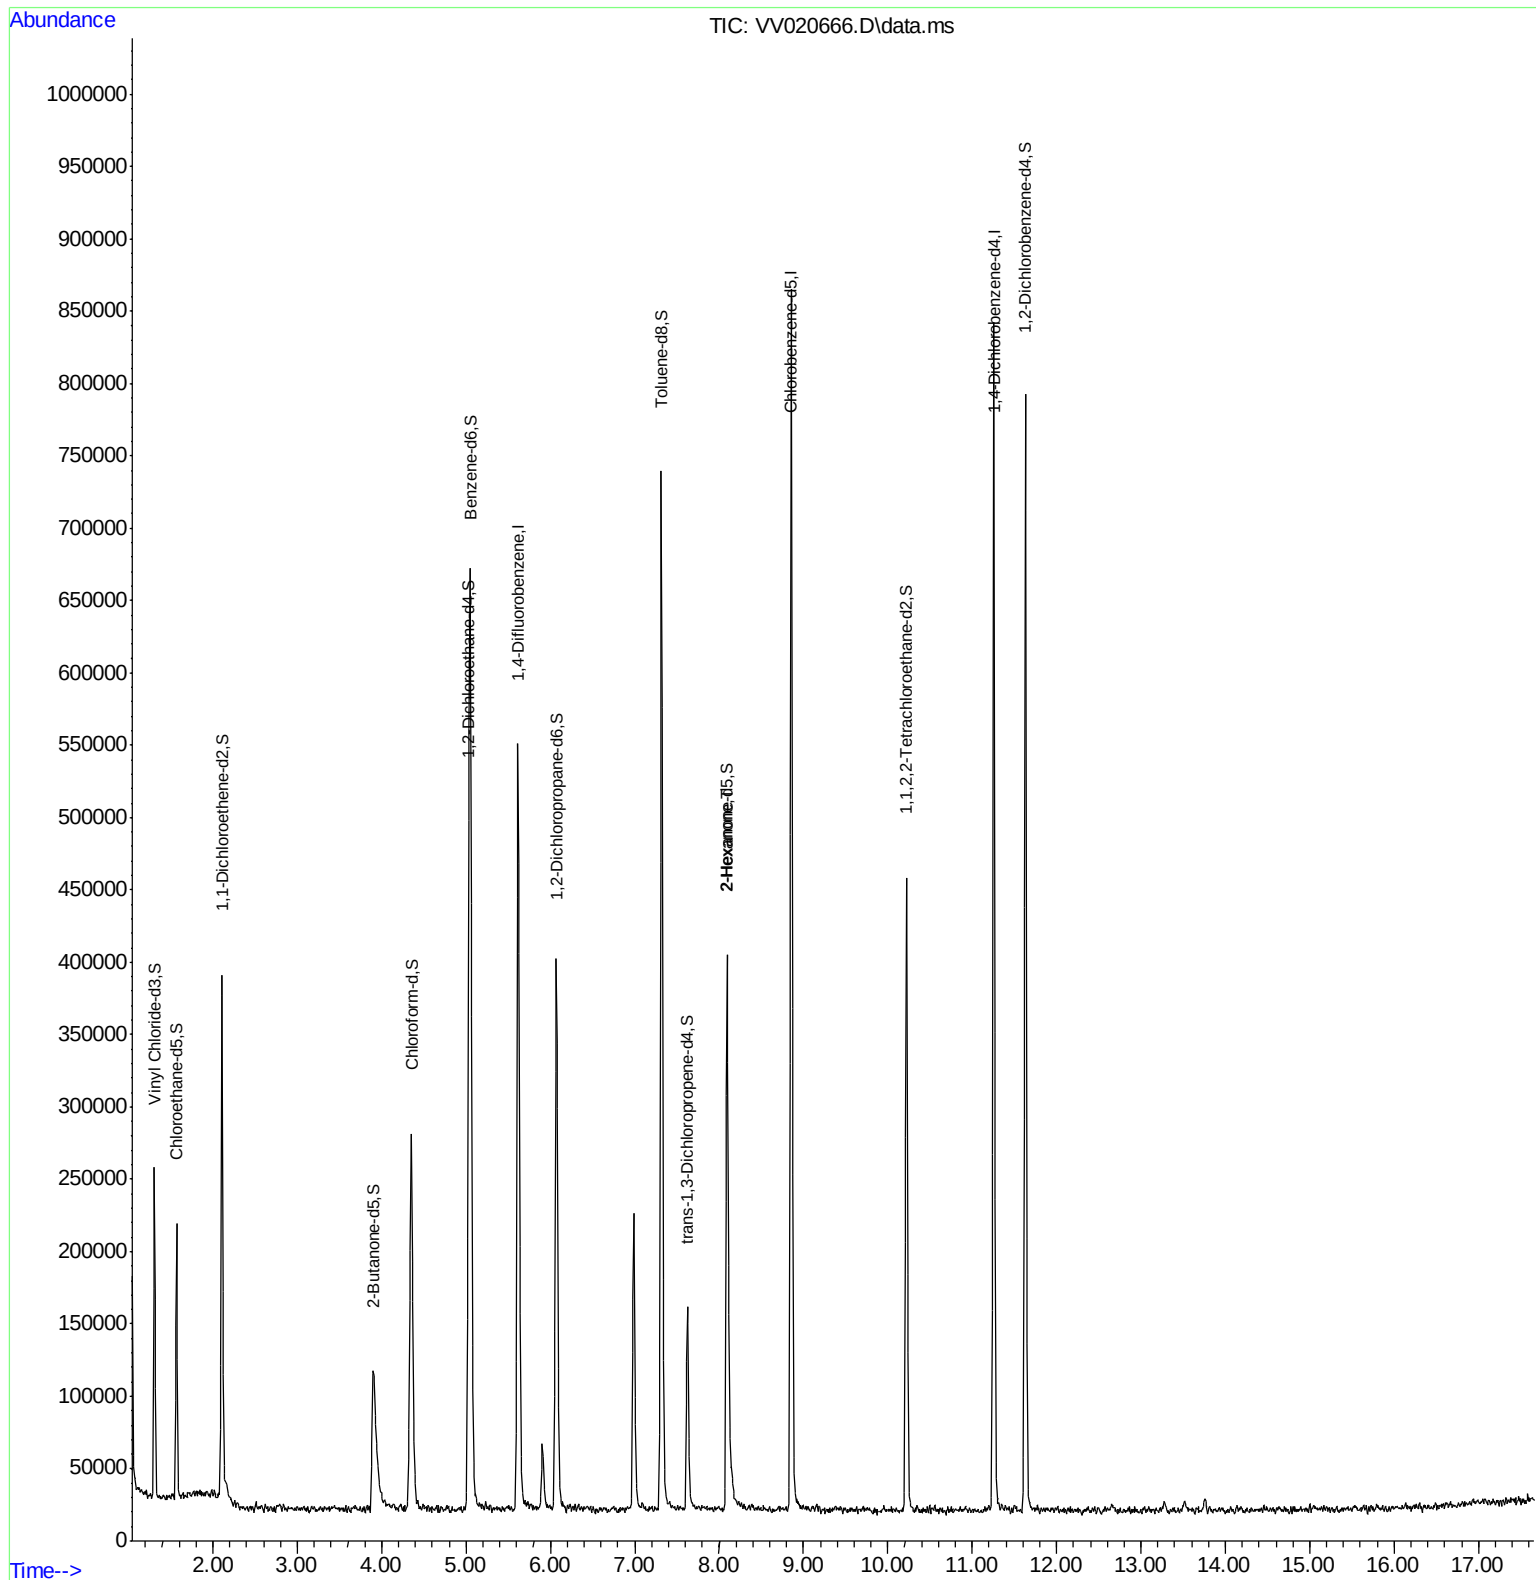

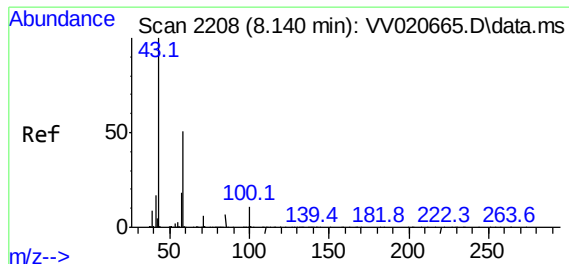

#48
 2-Hexanone
 Concen: 4.78 ug/L
 RT: 8.095 min Scan# 2194
 Delta R.T. -0.045 min
 Lab File: VV020666.D
 Acq: 18 Mar 2021 10:39

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

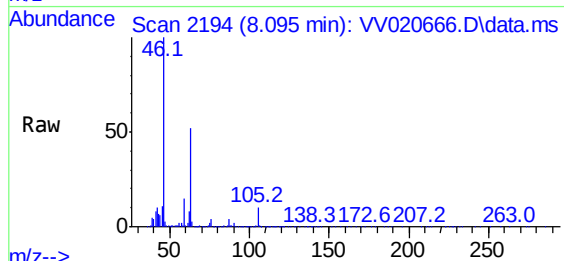

Tgt Ion: 43 Resp: 19296

Ion	Ratio	Lower	Upper
43	100		
58	0.0	41.8	62.6#
57	19.1	15.0	22.4
100	0.6	8.9	13.3#

