

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031919\
 Data File : VV009775.D
 Acq On : 19 Mar 2019 13:54
 Operator : SY/MD
 Sample : VV0319MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	79	rVB	54148	52989	13.50%	1.754%
2	2.122	313	321	336	rVB	104653	146081	37.20%	4.835%
3	2.450	421	423	425	rBV2	388	142	0.04%	0.005%
4	2.495	434	437	443	rBV	398	389	0.10%	0.013%
5	2.601	468	470	473	rBV	575	384	0.10%	0.013%
6	2.727	507	509	512	rBV	233	136	0.03%	0.005%
7	2.814	532	536	537	rBV	492	335	0.09%	0.011%
8	2.936	570	574	577	rBV	620	529	0.13%	0.018%
9	3.010	591	597	601	rBV2	663	751	0.19%	0.025%
10	3.029	601	603	606	rVB2	409	242	0.06%	0.008%
11	3.052	606	610	612	rBV	554	422	0.11%	0.014%
12	3.113	628	629	631	rVB	175	50	0.01%	0.002%
13	3.129	631	634	635	rBV	482	285	0.07%	0.009%
14	3.315	688	692	695	rBV	545	448	0.11%	0.015%
15	3.380	708	712	714	rBV2	580	537	0.14%	0.018%
16	3.473	739	741	743	rBV	293	185	0.05%	0.006%
17	3.502	748	750	751	rBV	323	168	0.04%	0.006%
18	3.579	770	774	777	rBV	304	294	0.07%	0.010%
19	3.627	784	789	792	rBV2	887	799	0.20%	0.026%
20	3.669	798	802	806	rVB	756	567	0.14%	0.019%
21	3.695	806	810	817	rBV	415	621	0.16%	0.021%
22	3.730	817	821	825	rBV2	634	613	0.16%	0.020%
23	3.788	834	839	841	rBV2	462	371	0.09%	0.012%
24	3.804	841	844	847	rBV	453	272	0.07%	0.009%
25	3.865	860	863	867	rBV	486	257	0.07%	0.009%
26	3.929	872	883	901	rBV	24343	62458	15.91%	2.067%
27	4.119	939	942	944	rBV2	674	457	0.12%	0.015%
28	4.177	957	960	965	rVB2	936	829	0.21%	0.027%
29	4.399	1015	1029	1048	rBV2	58475	139939	35.64%	4.631%
30	4.595	1088	1090	1092	rBV	193	88	0.02%	0.003%
31	4.608	1092	1094	1095	rBV	356	147	0.04%	0.005%
32	4.714	1122	1127	1132	rBV2	744	846	0.22%	0.028%
33	4.775	1143	1146	1151	rBV2	607	537	0.14%	0.018%
34	4.859	1169	1172	1175	rVB	506	267	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031919\
 Data File : VV009775.D
 Acq On : 19 Mar 2019 13:54
 Operator : SY/MD
 Sample : VV0319MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Title : VOC Analysis

35	4.897	1181	1184	1186	rBV2	460	297	0.08%	0.010%
36	5.016	1218	1221	1222	rBV	368	256	0.07%	0.008%
37	5.093	1227	1245	1262	rBV3	147032	364345	92.79%	12.058%
38	5.357	1323	1327	1330	rBV	782	489	0.12%	0.016%
39	5.392	1335	1338	1344	rVV2	890	786	0.20%	0.026%
40	5.482	1362	1366	1368	rBV	307	232	0.06%	0.008%
41	5.572	1391	1394	1396	rBV	551	364	0.09%	0.012%
42	5.662	1407	1422	1450	rBV2	152625	314034	79.98%	10.393%
43	6.116	1549	1563	1578	rBV2	80324	163334	41.60%	5.406%
44	6.280	1611	1614	1618	rBV2	683	554	0.14%	0.018%
45	6.325	1625	1628	1636	rBV	933	1036	0.26%	0.034%
46	6.360	1636	1639	1642	rBV	456	340	0.09%	0.011%
47	6.421	1656	1658	1661	rBV2	277	202	0.05%	0.007%
48	6.482	1674	1677	1682	rVB2	435	263	0.07%	0.009%
49	6.621	1718	1720	1724	rVB2	552	307	0.08%	0.010%
50	6.662	1729	1733	1735	rBV	755	571	0.15%	0.019%
51	6.701	1740	1745	1751	rVB2	1295	1300	0.33%	0.043%
52	6.904	1804	1808	1811	rBV2	548	454	0.12%	0.015%
53	6.952	1820	1823	1825	rBV2	573	442	0.11%	0.015%
54	7.029	1836	1847	1859	rBV	46680	82619	21.04%	2.734%
55	7.238	1910	1912	1915	rBV	410	207	0.05%	0.007%
56	7.277	1922	1924	1926	rBV	437	220	0.06%	0.007%
57	7.360	1938	1950	1976	rBV	172114	311535	79.34%	10.311%
58	7.662	2035	2044	2059	rVB	30656	51986	13.24%	1.721%
59	7.836	2092	2098	2101	rBV	562	716	0.18%	0.024%
60	7.871	2105	2109	2114	rBV2	598	635	0.16%	0.021%
61	8.135	2180	2191	2210	rBV	75728	148102	37.72%	4.902%
62	8.354	2255	2259	2261	rBV	661	507	0.13%	0.017%
63	8.466	2291	2294	2297	rBV	391	327	0.08%	0.011%
64	8.794	2393	2396	2398	rBV	465	304	0.08%	0.010%
65	8.897	2415	2428	2451	rBV	232686	392654	100.00%	12.995%
66	9.045	2470	2474	2479	rBV	572	669	0.17%	0.022%
67	9.145	2503	2505	2509	rVB	509	288	0.07%	0.010%
68	9.203	2520	2523	2526	rBV	469	325	0.08%	0.011%
69	9.585	2638	2642	2643	rBV	726	524	0.13%	0.017%
70	9.694	2673	2676	2677	rBV2	275	164	0.04%	0.005%
71	9.730	2685	2687	2690	rBV	635	363	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV031919\
 Data File : VV009775.D
 Acq On : 19 Mar 2019 13:54
 Operator : SY/MD
 Sample : VV0319MBL01
 Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Title : VOC Analysis

72	9.878	2729	2733	2734	rBV	576	460	0.12%	0.015%
73	10.222	2837	2840	2842	rBV	522	266	0.07%	0.009%
74	10.264	2842	2853	2873	rVV	118178	191399	48.74%	6.335%
75	10.476	2916	2919	2922	rBV	538	426	0.11%	0.014%
76	10.518	2929	2932	2934	rBV	546	297	0.08%	0.010%
77	10.601	2954	2958	2961	rBV	827	692	0.18%	0.023%
78	10.765	3007	3009	3012	rBV	472	346	0.09%	0.011%
79	10.955	3061	3068	3072	rBV	753	869	0.22%	0.029%
80	11.299	3163	3175	3191	rBV	178952	311080	79.22%	10.296%
81	11.534	3245	3248	3251	rBV	515	309	0.08%	0.010%
82	11.675	3280	3292	3307	rBV	148308	253156	64.47%	8.378%
83	11.894	3358	3360	3362	rBV	548	253	0.06%	0.008%
84	12.125	3428	3432	3434	rBV2	742	535	0.14%	0.018%
85	12.283	3478	3481	3484	rBV	593	456	0.12%	0.015%
86	12.434	3525	3528	3530	rBV	562	290	0.07%	0.010%
87	13.093	3731	3733	3736	rBV	573	367	0.09%	0.012%
88	13.235	3773	3777	3780	rBV	847	811	0.21%	0.027%
89	13.273	3786	3789	3791	rBV	654	459	0.12%	0.015%
90	13.498	3856	3859	3862	rBV	762	607	0.15%	0.020%
91	13.620	3895	3897	3898	rBV	415	190	0.05%	0.006%
92	13.778	3944	3946	3949	rBV	586	394	0.10%	0.013%
93	14.167	4063	4067	4072	rBV3	845	1067	0.27%	0.035%
94	14.443	4151	4153	4155	rBV2	667	349	0.09%	0.012%
95	14.691	4226	4230	4236	rBV2	887	1245	0.32%	0.041%


Sum of corrected areas: 3021509

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV031919\
Data File : VV009775.D
Acq On : 19 Mar 2019 13:54
Operator : SY/MD
Sample : VV0319MBL01
Misc : 5.0µL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

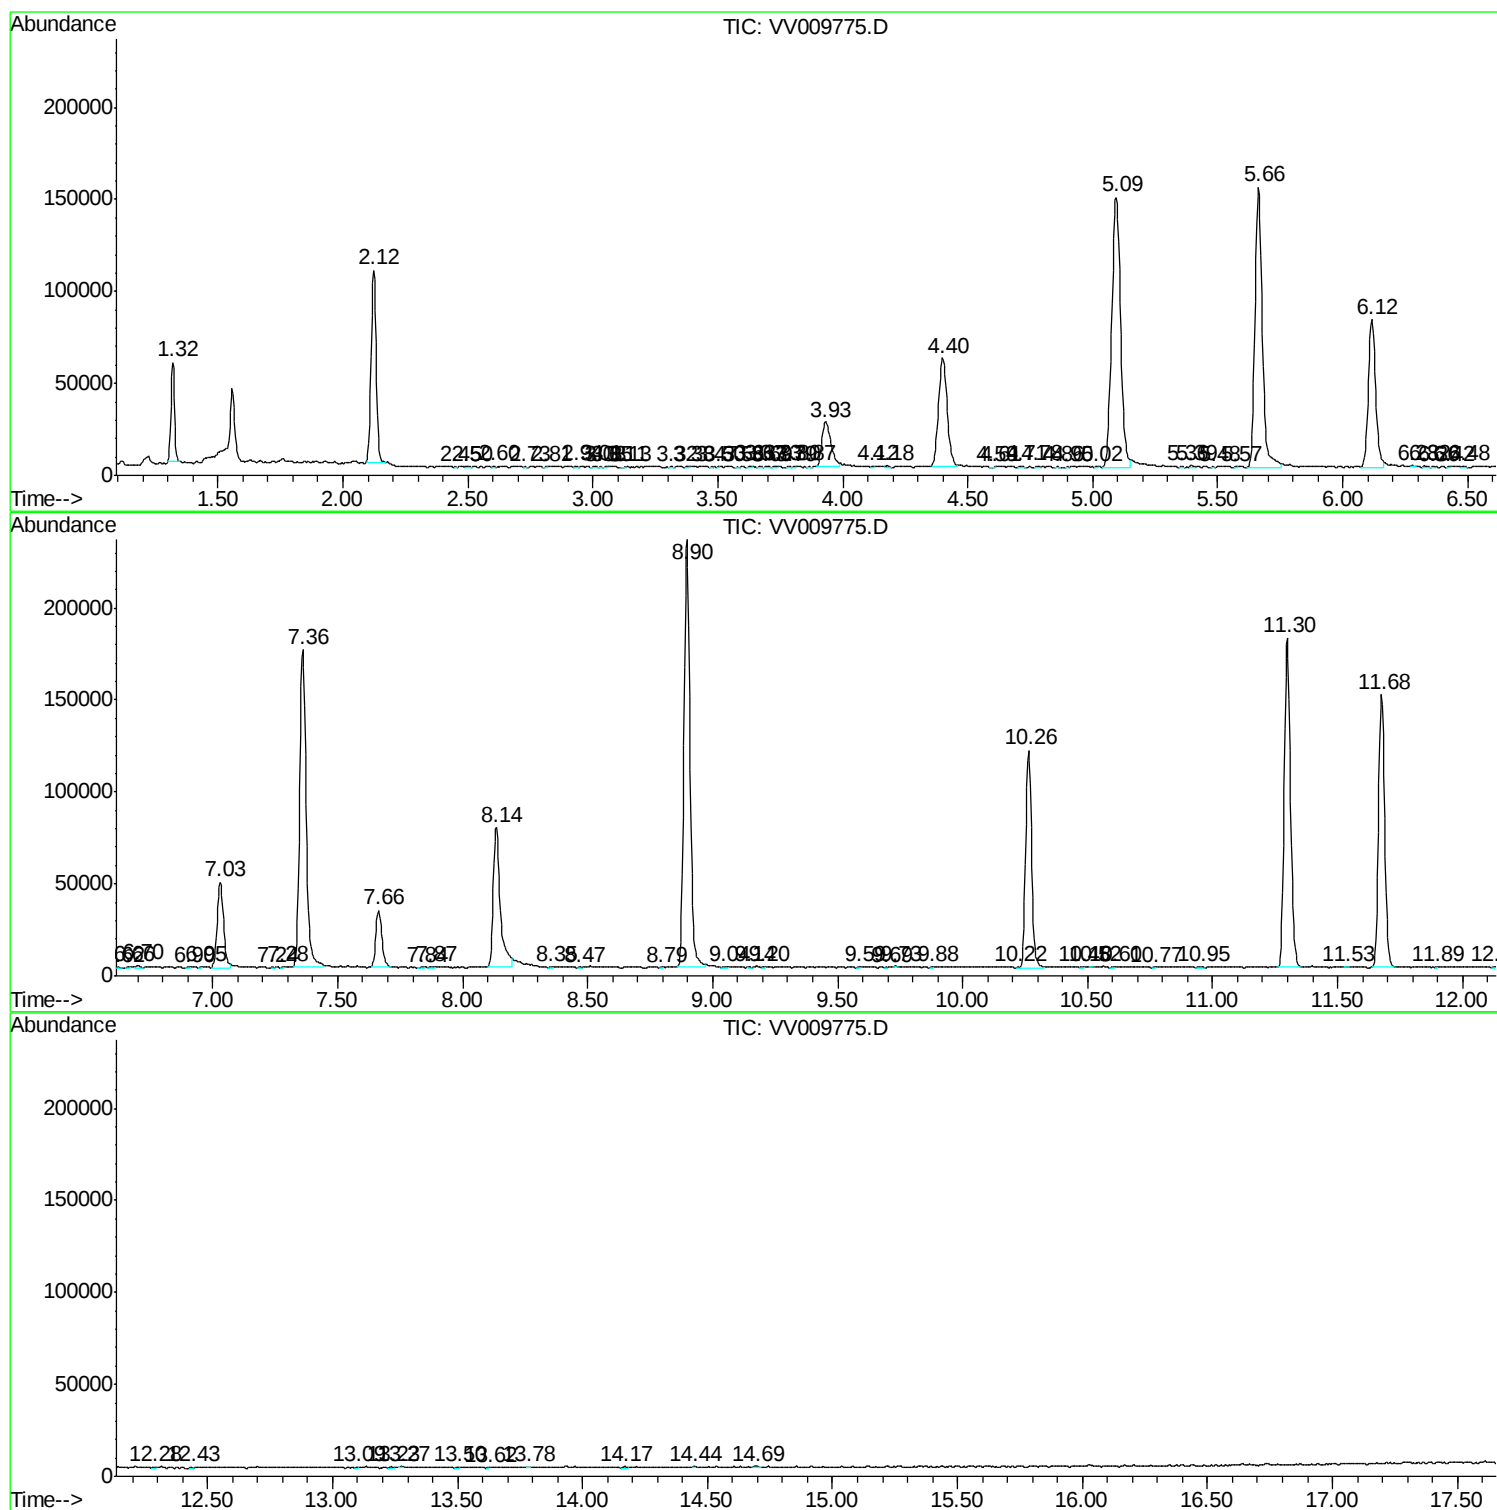

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031919\
Data File : VV009775.D
Acq On : 19 Mar 2019 13:54
Operator : SY/MD
Sample : VV0319MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV031919\
Data File : VV009775.D
Acq On : 19 Mar 2019 13:54
Operator : SY/MD
Sample : VV0319MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc