


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV031919\
 Data File : VV009773.D
 Acq On : 19 Mar 2019 09:16
 Operator : SY/MD
 Sample : BFB81
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM031719WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 20 05:16:13 2019

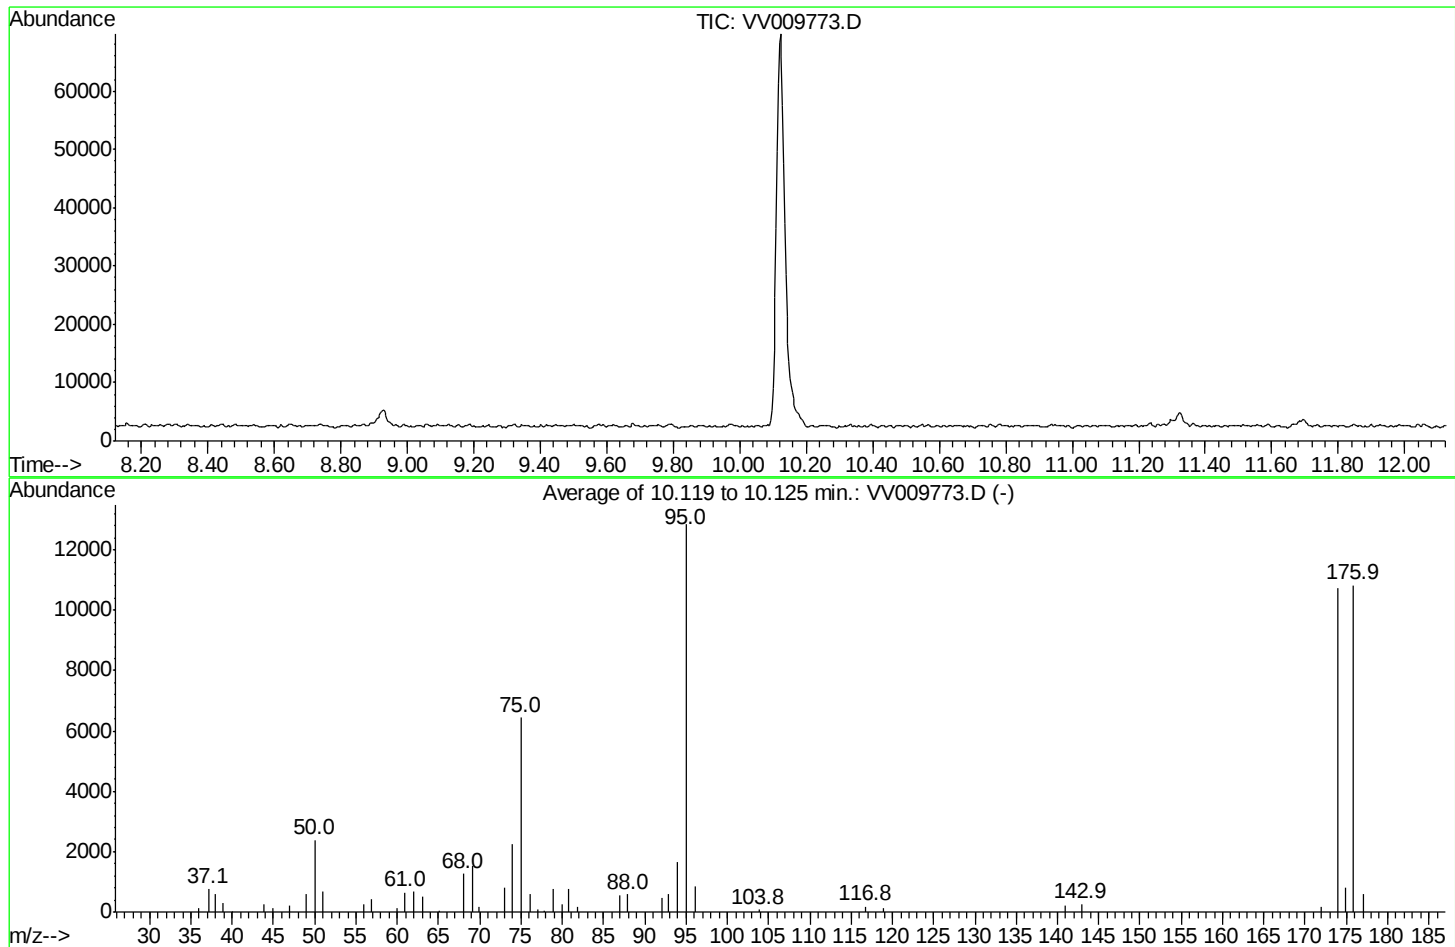

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	2383	PASS
75	95	30	80	50.1	6431	PASS
95	95	100	100	100.0	12844	PASS
96	95	5	9	6.7	866	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.6	10742	PASS
175	174	5	9	7.7	824	PASS
176	174	95	101	100.7	10819	PASS
177	176	5	9	5.7	612	PASS

Scan 2798 (10.087 min): VV009773.D
BFB81

m/z	Abundance
40.00	2495.0
44.10	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	139.0
37.10	724.0
38.00	583.0
38.90	281.0
40.00	2498.0
43.90	279.0
45.10	109.0
47.00	174.0
48.90	638.0
50.00	2443.0
51.00	737.0
56.00	286.0
56.90	442.0
60.00	139.0
60.90	614.0
62.00	764.0
63.00	491.0
68.00	1311.0
69.00	1565.0
70.00	177.0
73.00	795.0
74.00	2332.0
75.00	6466.0
76.10	621.0
77.00	145.0
78.90	804.0
80.00	225.0
80.80	779.0
81.90	183.0
86.90	567.0
87.90	518.0
92.10	499.0
92.90	598.0
94.00	1741.0
95.00	12703.0
96.00	834.0
103.80	117.0
116.80	151.0
119.00	127.0
140.90	235.0
142.90	270.0
171.90	119.0
174.00	10633.0
175.00	824.0
175.90	10861.0
177.00	677.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.90	116.0
37.10	805.0
38.00	604.0
38.90	338.0
39.90	2495.0
43.90	252.0
45.00	120.0
47.00	215.0
49.00	582.0
50.00	2468.0
51.00	725.0
56.00	262.0
56.90	438.0
60.00	136.0
61.00	671.0
62.00	690.0
63.10	555.0
68.00	1294.0
69.10	1559.0
69.90	175.0
73.00	832.0
74.00	2365.0
75.00	6636.0
76.00	592.0
77.00	130.0
78.80	783.0
80.00	234.0
80.80	787.0
81.90	190.0
86.90	595.0
88.00	473.0
92.10	492.0
92.90	640.0
94.00	1689.0
95.00	13241.0
96.10	877.0
103.80	103.0
116.80	198.0
118.90	130.0
140.90	234.0
142.90	288.0
172.00	156.0
174.00	11085.0
175.00	844.0
175.90	11100.0
177.00	611.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
35.80	128.0
37.10	780.0
38.00	594.0
39.00	328.0
39.90	2534.0
43.80	263.0
44.90	109.0
47.00	273.0
49.00	565.0
50.00	2238.0
51.00	642.0
55.90	240.0
56.90	374.0
60.00	161.0
61.00	643.0
62.00	624.0
63.00	522.0
65.10	101.0
68.00	1185.0
69.10	1442.0
69.90	171.0
73.00	748.0
74.00	2115.0
75.00	6193.0
76.00	536.0
77.80	120.0
78.80	656.0
80.00	247.0
80.80	705.0
81.90	158.0
87.00	532.0
87.80	366.0
88.00	372.0
92.10	388.0
92.90	568.0
94.00	1528.0
95.00	12590.0
96.10	887.0
116.80	209.0
118.90	121.0
140.90	204.0
142.90	234.0
172.00	177.0
174.00	10510.0
174.90	806.0
175.90	10496.0
177.00	549.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81