

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031921\
 Data File : VV020688.D
 Acq On : 19 Mar 2021 14:17
 Operator : SY/MD
 Sample : M1698-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK75

Quant Time: Mar 20 00:21:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 20 00:20:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	382482	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	383821	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	174630	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	180961	58.65	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 117.30%			
7) Chloroethane-d5	1.571	69	130501	52.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 105.74%			
11) 1,1-Dichloroethene-d2	2.108	63	236095	40.26	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 80.52%			
21) 2-Butanone-d5	3.889	46	204273	103.16	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 103.16%			
24) Chloroform-d	4.349	84	301869	56.29	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 112.58%			
26) 1,2-Dichloroethane-d4	5.034	65	196862	55.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 111.28%			
32) Benzene-d6	5.050	84	582191	54.90	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 109.80%			
36) 1,2-Dichloropropane-d6	6.072	67	184384	54.35	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 108.70%			
41) Toluene-d8	7.317	98	505669	53.65	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 107.30%			
43) trans-1,3-Dichloroprop...	7.622	79	88624	55.89	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 111.78%			
47) 2-Hexanone-d5	8.091	63	137476	108.30	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 108.30%			
57) 1,1,2,2-Tetrachloroeth...	10.220	84	239467	56.48	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 112.96%			
64) 1,2-Dichlorobenzene-d4	11.628	152	191571	56.61	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 113.22%			
Target Compounds					Qvalue	
13) Acetone	2.188	43	10906	6.74	ug/L	63
59) 1,2,3-Trichloropropane	11.255	75	24473	6.39	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031921\
Data File : VV020688.D
Acq On : 19 Mar 2021 14:17
Operator : SY/MD
Sample : M1698-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK75

Quant Time: Mar 20 00:21:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 20 00:20:14 2021
Response via : Initial Calibration




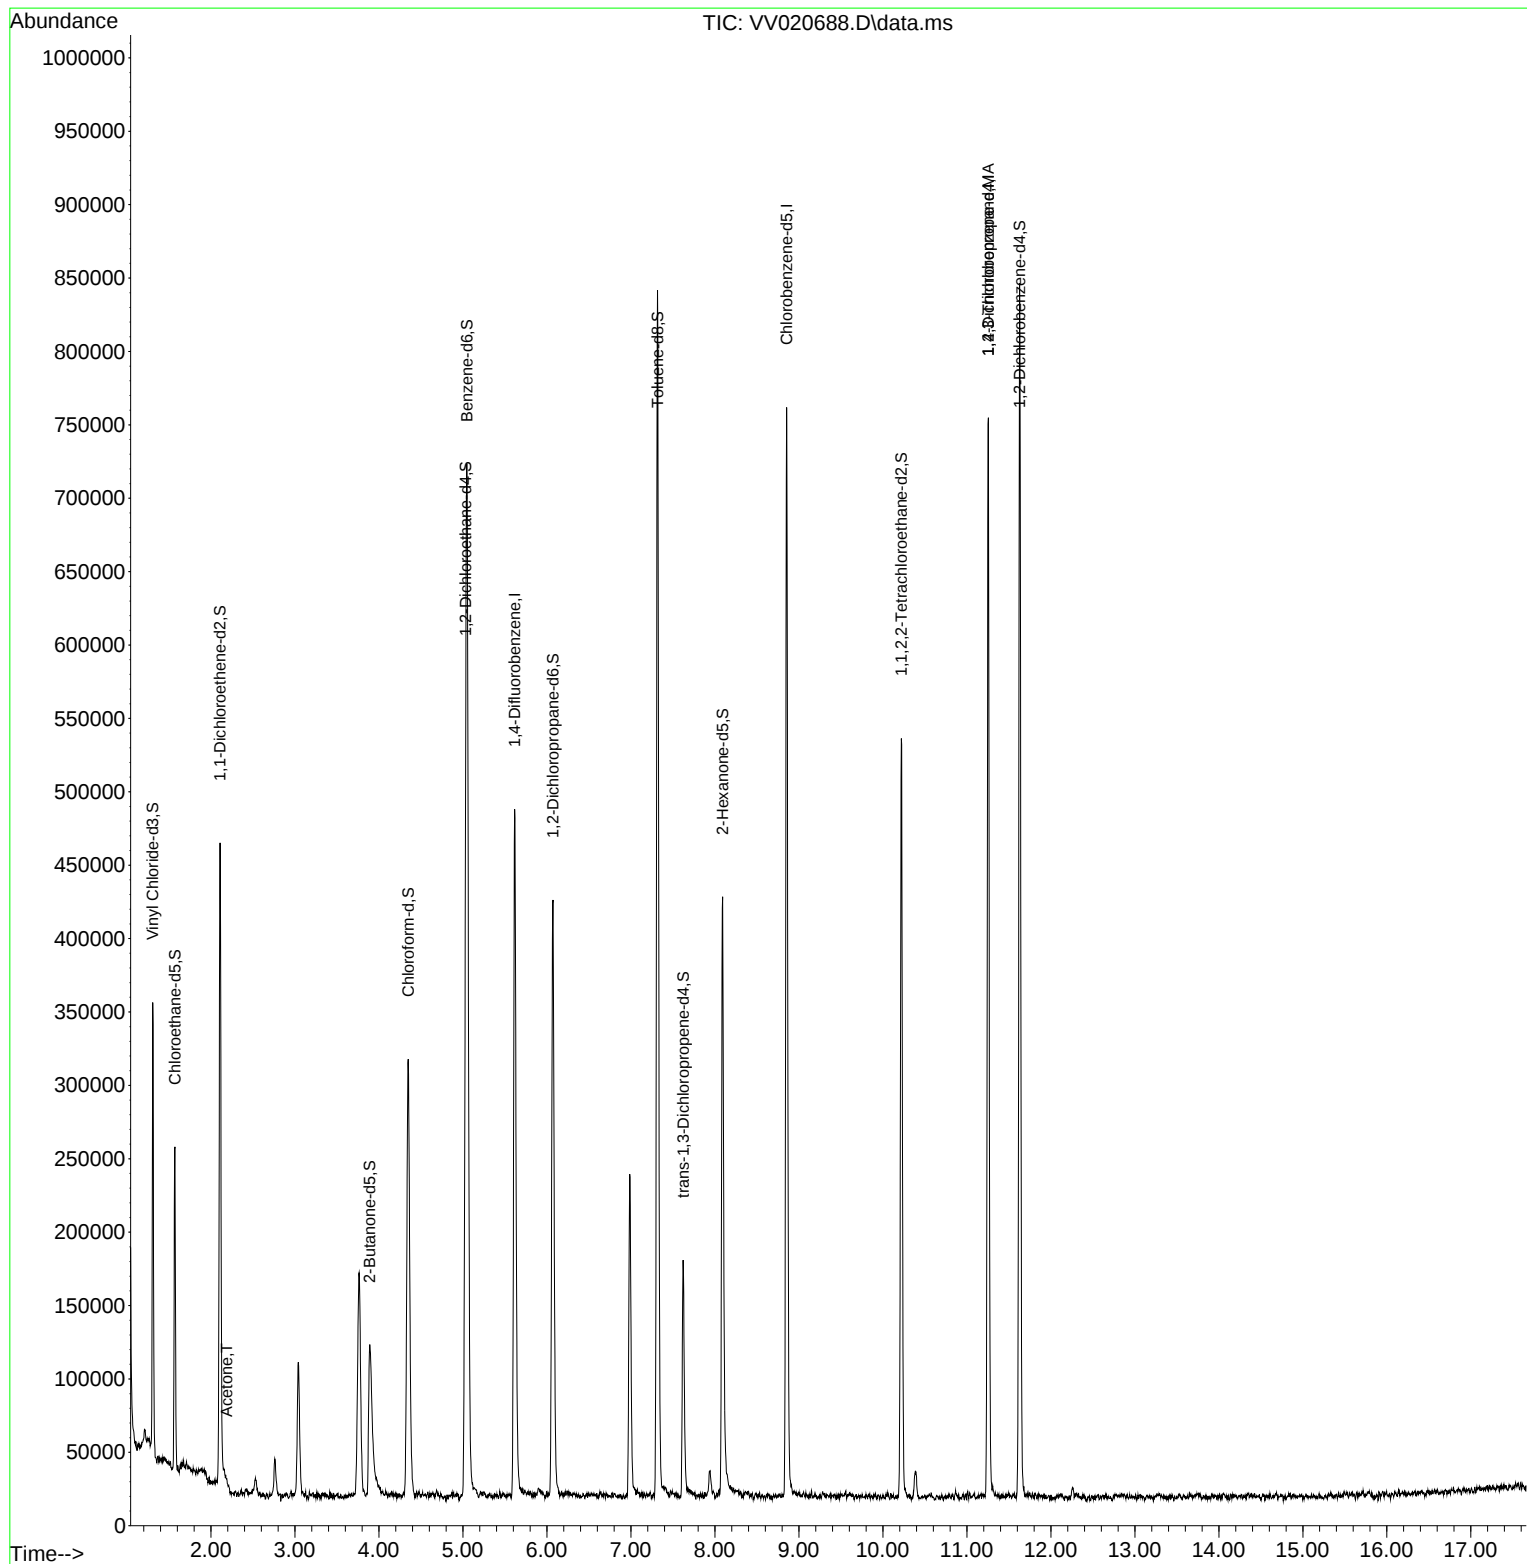


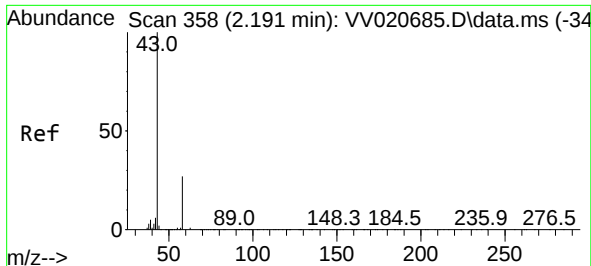

#13
Acetone
Concen: 6.74 ug/L
RT: 2.188 min Scan# 357
Delta R.T. -0.003 min
Lab File: VV020688.D
Acq: 19 Mar 2021 14:17

Instrument :
MSVOA_V
ClientSampled :
VBLK75

Tgt Ion: 43 Resp: 10906
Ion Ratio Lower Upper
43 100
58 9.9 0.0 60.2

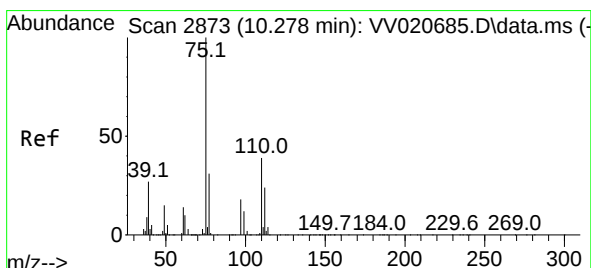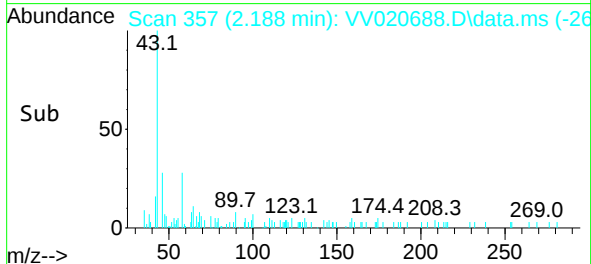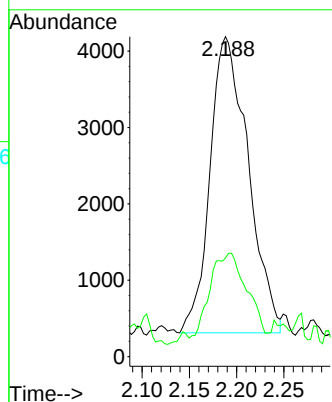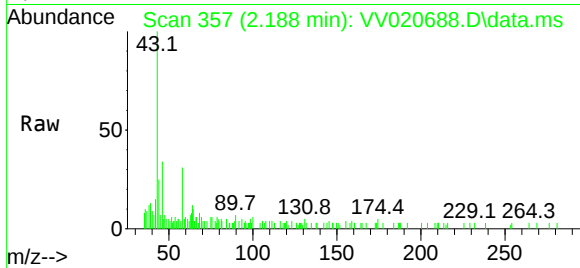

#59
1,2,3-Trichloropropane
Concen: 6.39 ug/L
RT: 11.255 min Scan# 3177
Delta R.T. 0.977 min
Lab File: VV020688.D
Acq: 19 Mar 2021 14:17

Tgt Ion: 75 Resp: 24473
Ion Ratio Lower Upper
75 100
77 37.6 25.4 38.0

