

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031921\
 Data File : VV020691.D
 Acq On : 19 Mar 2021 15:58
 Operator : SY/MD
 Sample : M1698-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M

Title : VOC Analysis

Signal : TIC: VV020691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	91	rVB	282239	275886	16.92%	2.213%
2	1.571	159	165	174	rVB	213512	231767	14.21%	1.859%
3	2.111	325	333	355	rVB	409046	616654	37.82%	4.945%
4	3.053	624	626	632	rBV7	3345	3565	0.22%	0.029%
5	3.153	655	657	660	rBV4	2843	1580	0.10%	0.013%
6	3.596	788	795	798	rBV9	5503	7078	0.43%	0.057%
7	3.886	877	885	908	rBV	97181	269335	16.52%	2.160%
8	4.294	1005	1012	1014	rBV8	5770	7046	0.43%	0.057%
9	4.349	1018	1029	1048	rVB2	267590	660557	40.51%	5.297%
10	4.802	1168	1170	1171	rBV2	2717	1309	0.08%	0.010%
11	4.934	1207	1211	1213	rBV4	2746	2055	0.13%	0.016%
12	4.947	1213	1215	1217	rBV3	3476	2386	0.15%	0.019%
13	5.047	1231	1246	1267	rBV2	650774	1630695	100.00%	13.078%
14	5.468	1375	1377	1378	rBV2	1978	560	0.03%	0.004%
15	5.529	1392	1396	1398	rBV5	3444	2913	0.18%	0.023%
16	5.619	1413	1424	1442	rBV	483477	946919	58.07%	7.594%
17	6.072	1554	1565	1586	rVB2	377144	741770	45.49%	5.949%
18	6.616	1731	1734	1736	rBV3	3591	2670	0.16%	0.021%
19	6.989	1840	1850	1865	rBV	199736	357922	21.95%	2.870%
20	7.317	1942	1952	1972	rBV	757976	1282924	78.67%	10.289%
21	7.622	2039	2047	2063	rBV	142398	242298	14.86%	1.943%
22	8.091	2183	2193	2218	rBV	388606	709552	43.51%	5.690%
23	8.320	2261	2264	2266	rBV4	3748	2960	0.18%	0.024%
24	8.853	2420	2430	2448	rBV	783301	1244073	76.29%	9.977%
25	9.268	2557	2559	2560	rBV2	3290	1436	0.09%	0.012%
26	9.455	2611	2617	2618	rBV6	3218	3226	0.20%	0.026%
27	9.799	2722	2724	2728	rVB5	3527	2179	0.13%	0.017%
28	10.095	2814	2816	2818	rBV3	3344	1463	0.09%	0.012%
29	10.220	2844	2855	2868	rBV	506914	775749	47.57%	6.221%
30	10.320	2884	2886	2889	rBV3	3560	2310	0.14%	0.019%
31	10.516	2945	2947	2949	rBV3	2371	1404	0.09%	0.011%
32	10.625	2978	2981	2983	rBV4	2942	2229	0.14%	0.018%
33	10.651	2987	2989	2990	rBV2	2538	1009	0.06%	0.008%
34	10.783	3026	3030	3031	rBV4	3528	2347	0.14%	0.019%
35	10.831	3043	3045	3046	rBV2	1995	876	0.05%	0.007%
36	10.947	3079	3081	3083	rBV3	4499	2505	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031921\
 Data File : VV020691.D
 Acq On : 19 Mar 2021 15:58
 Operator : SY/MD
 Sample : M1698-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
 Title : VOC Analysis

37	11.104	3127	3130	3131	rBV3	3865	2286	0.14%	0.018%
38	11.143	3140	3142	3145	rBV4	2684	1185	0.07%	0.010%
39	11.255	3163	3177	3192	rBV	761772	1186398	72.75%	9.515%
40	11.541	3263	3266	3269	rBV4	4245	2790	0.17%	0.022%
41	11.580	3276	3278	3279	rBV2	1882	667	0.04%	0.005%
42	11.628	3282	3293	3307	rBV	769980	1191148	73.05%	9.553%
43	11.802	3345	3347	3349	rBV3	3535	1984	0.12%	0.016%
44	12.426	3538	3541	3542	rBV3	2518	1516	0.09%	0.012%
45	12.628	3599	3604	3605	rBV5	4476	2948	0.18%	0.024%
46	12.693	3622	3624	3625	rBV2	2784	1198	0.07%	0.010%
47	12.998	3716	3719	3721	rBV4	3582	2440	0.15%	0.020%
48	13.152	3765	3767	3770	rBV4	2774	1313	0.08%	0.011%
49	13.210	3783	3785	3786	rBV2	2742	1050	0.06%	0.008%
50	13.426	3850	3852	3853	rBV	3144	1537	0.09%	0.012%
51	13.451	3858	3860	3868	rVB8	4302	4182	0.26%	0.034%
52	13.545	3886	3889	3891	rBV4	2897	1714	0.11%	0.014%
53	13.815	3971	3973	3975	rBV3	2142	989	0.06%	0.008%
54	13.934	4009	4010	4013	rBV3	1930	1080	0.07%	0.009%
55	14.001	4028	4031	4034	rBV5	4256	2820	0.17%	0.023%
56	14.056	4046	4048	4052	rBV5	2169	1929	0.12%	0.015%
57	14.319	4128	4130	4131	rBV2	3411	1272	0.08%	0.010%
58	14.397	4150	4154	4157	rBV6	4633	3837	0.24%	0.031%
59	15.213	4404	4408	4410	rBV5	6014	4598	0.28%	0.037%
60	15.278	4427	4428	4430	rBV2	3179	1086	0.07%	0.009%
61	16.307	4746	4748	4752	rBV4	4269	3167	0.19%	0.025%
62	16.435	4786	4788	4791	rBV3	4511	3004	0.18%	0.024%




Sum of corrected areas: 12469345

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031921\
Data File : VV020691.D
Acq On : 19 Mar 2021 15:58
Operator : SY/MD
Sample : M1698-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

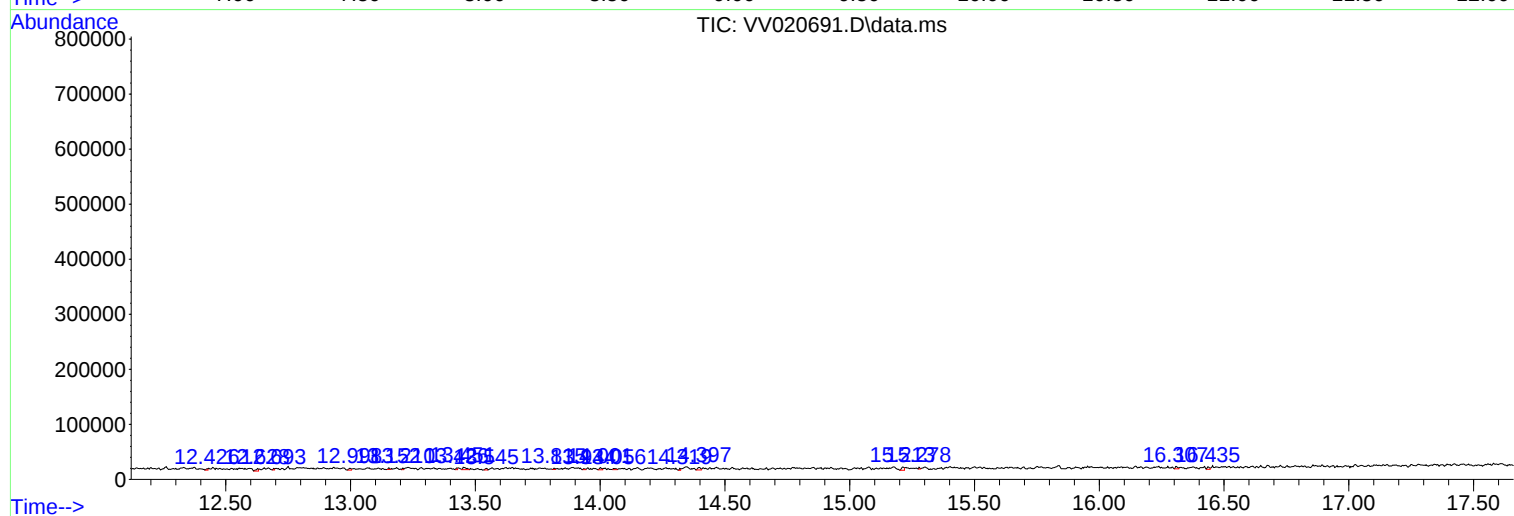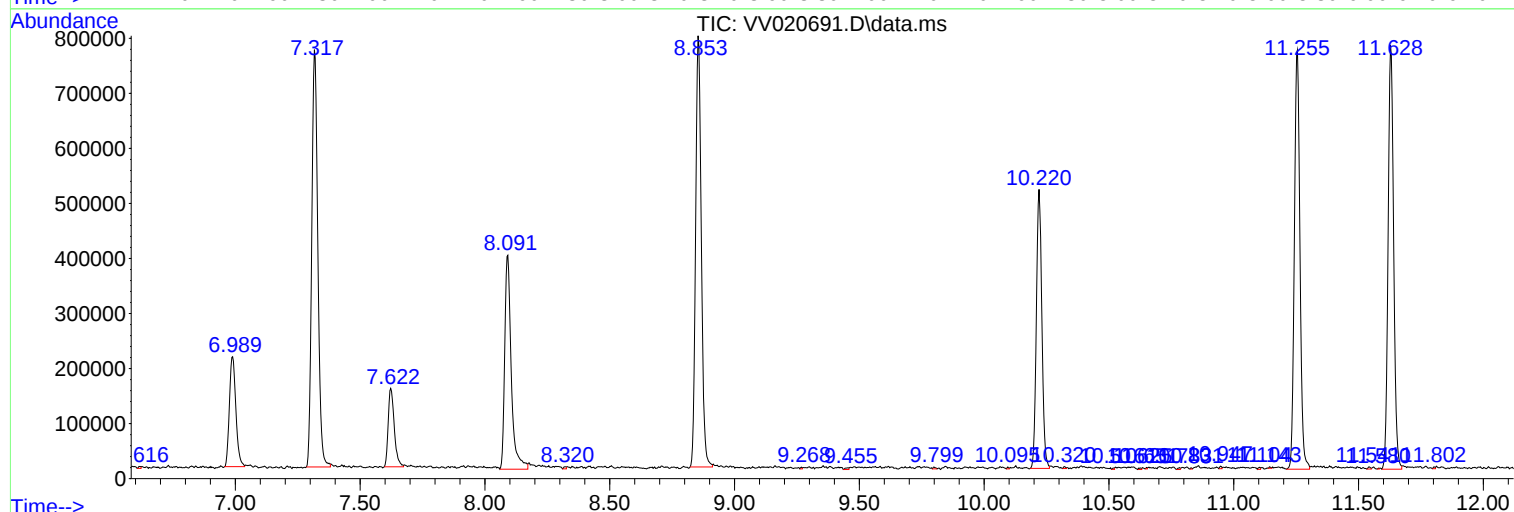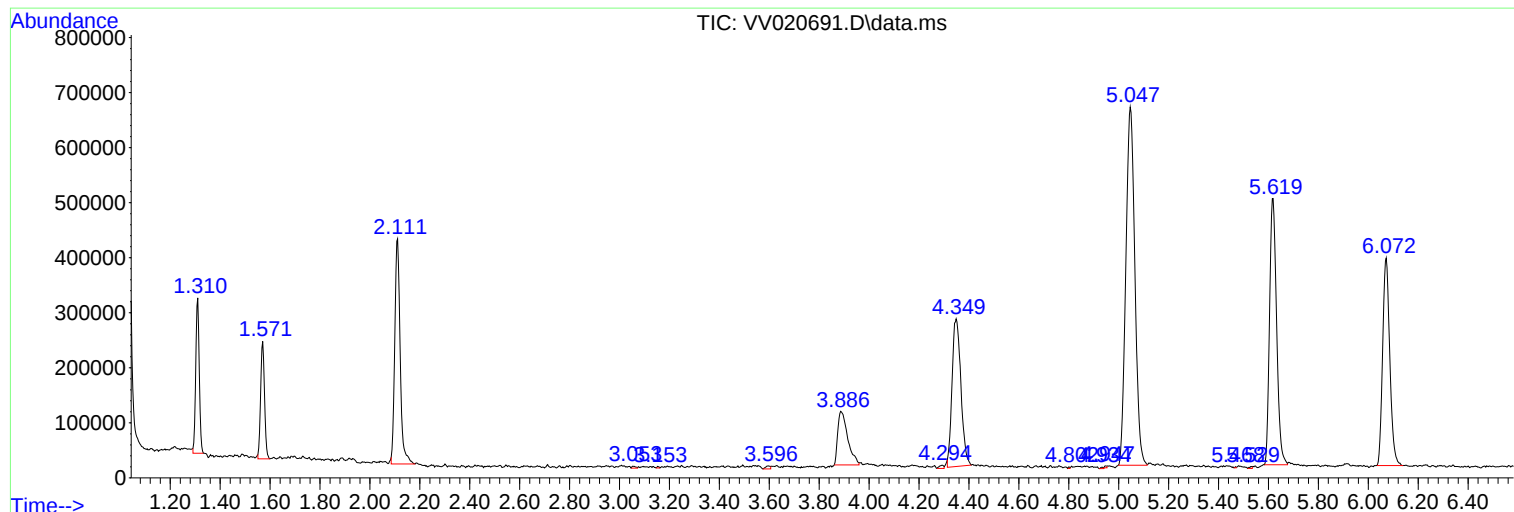

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031921\
Data File : VV020691.D
Acq On : 19 Mar 2021 15:58
Operator : SY/MD
Sample : M1698-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031921\
Data File : VV020691.D
Acq On : 19 Mar 2021 15:58
Operator : SY/MD
Sample : M1698-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM031321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
