

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034696.D
 Acq On : 18 Mar 2024 15:07
 Operator : SY/MD
 Sample : VV0318WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 19 02:54:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 19 02:53:17 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.535	114	369174	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.783	117	339903	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.185	152	167861	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	165264	51.639	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	103.280%	
7) Chloroethane-d5		1.532	69	127426	51.107	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.220%	
11) 1,1-Dichloroethene-d2		2.060	65	70904	48.989	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.980%	
21) 2-Butanone-d5		3.793	46	208414	97.381	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.380%	
24) Chloroform-d		4.249	84	272591	48.173	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.340%	
26) 1,2-Dichloroethane-d4		4.940	65	187011	50.574	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.140%	
32) Benzene-d6		4.960	84	546612	53.285	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.560%	
36) 1,2-Dichloropropane-d6		5.989	67	168028	53.672	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.340%	
41) Toluene-d8		7.243	98	492876	53.092	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.180%	
43) trans-1,3-Dichloroprop...		7.555	79	79181	50.366	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.740%	
47) 2-Hexanone-d5		8.024	63	127855	81.785	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.780%	
56) 1,1,2,2-Tetrachloroeth...		10.152	84	209226	50.784	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.560%	
66) 1,2-Dichlorobenzene-d4		11.558	152	183963	53.616	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.240%	
Target Compounds							Qvalue
61) 1,2,3-Trichloropropane		11.185	75	20012	6.245	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034696.D
Acq On : 18 Mar 2024 15:07
Operator : SY/MD
Sample : VV0318WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 19 02:54:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 19 02:53:17 2024
Response via : Initial Calibration

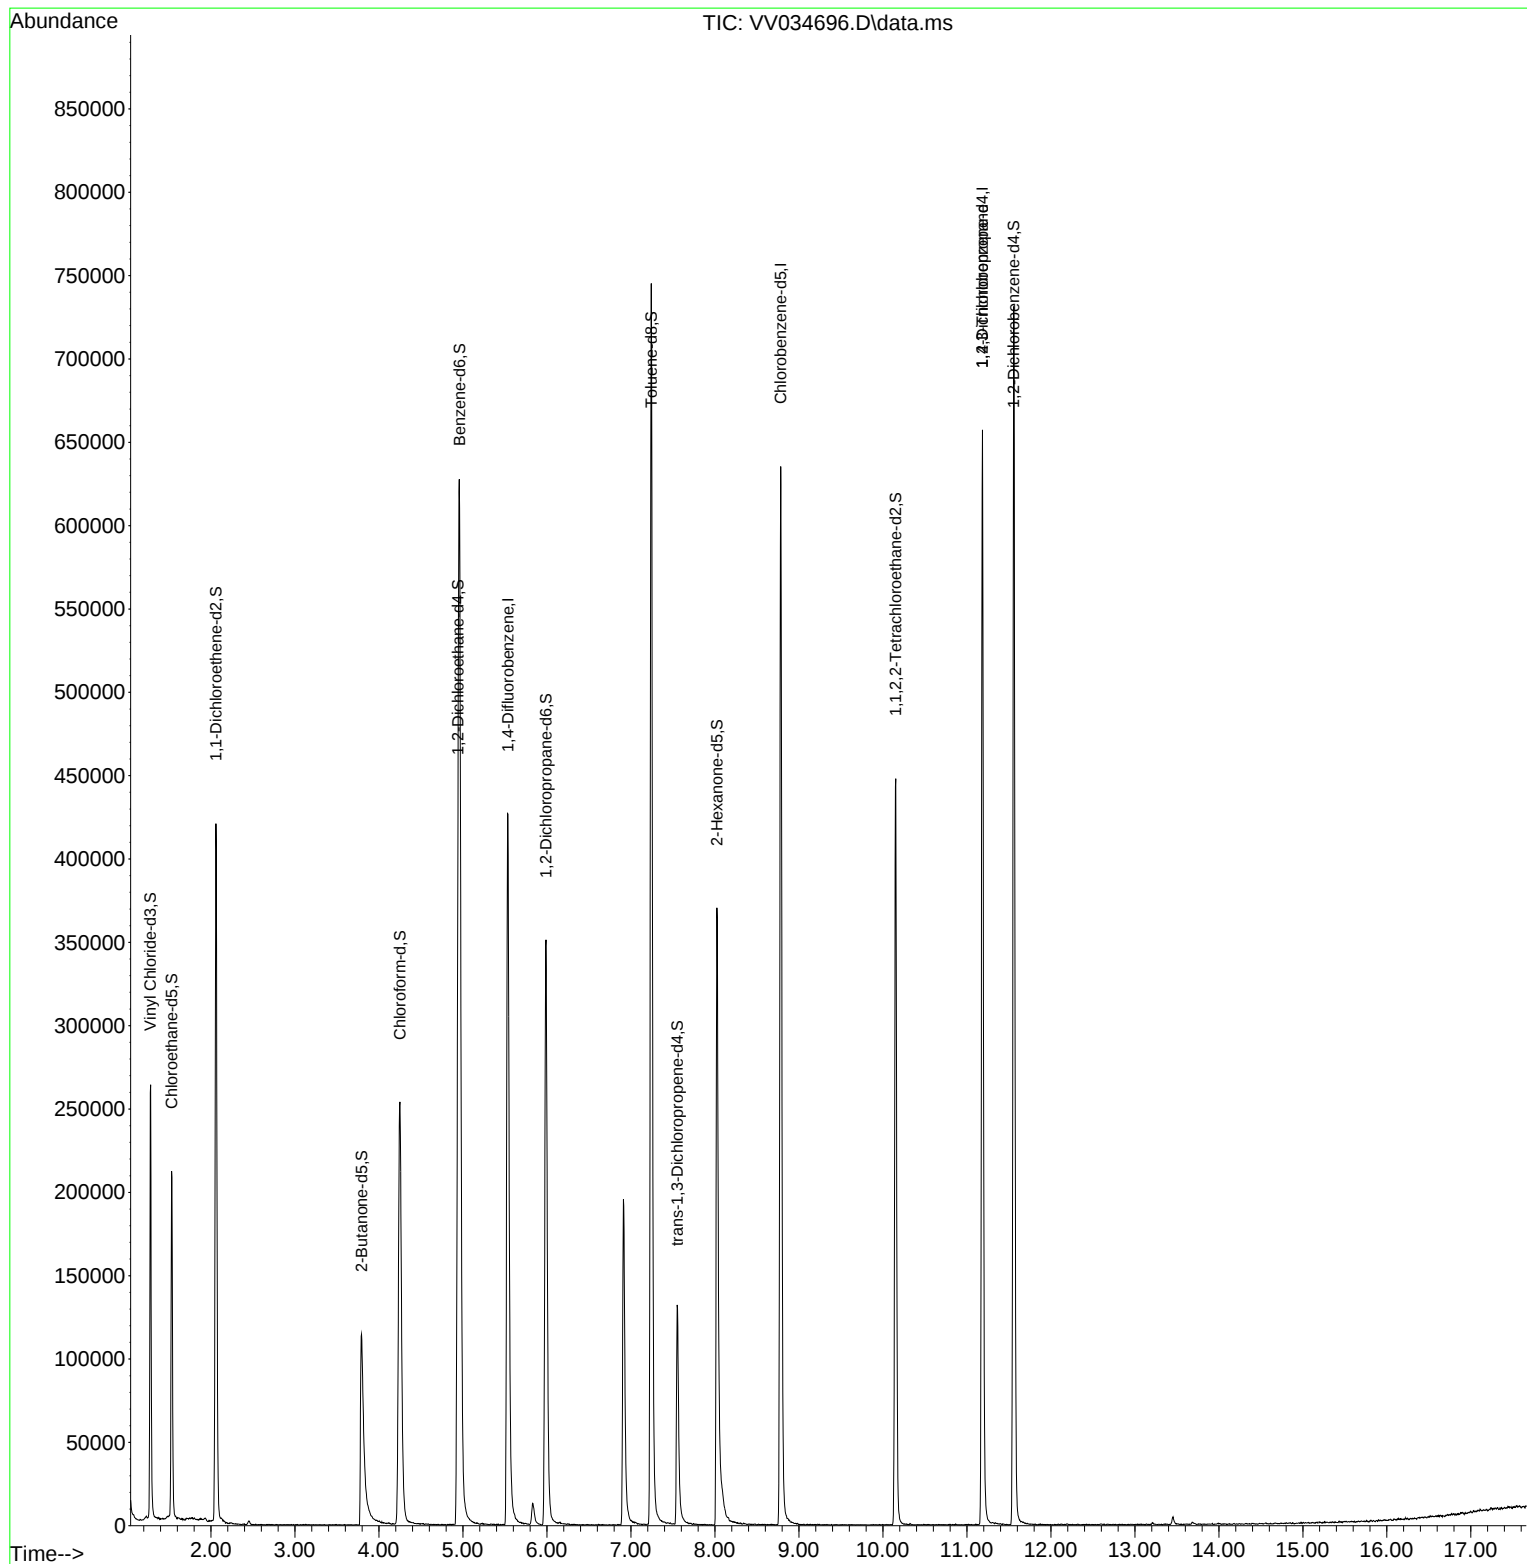

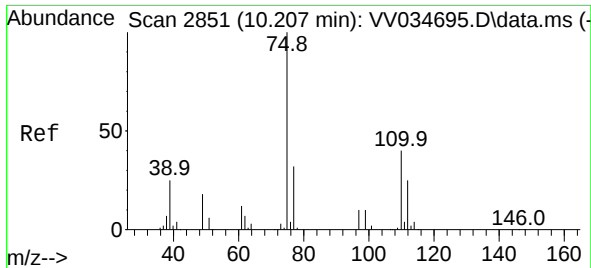

#61
 1,2,3-Trichloropropane
 Concen: 6.245 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.978 min
 Lab File: VV034696.D
 Acq: 18 Mar 2024 15:07

Instrument :
 MSVOA_V
 ClientSampleId :

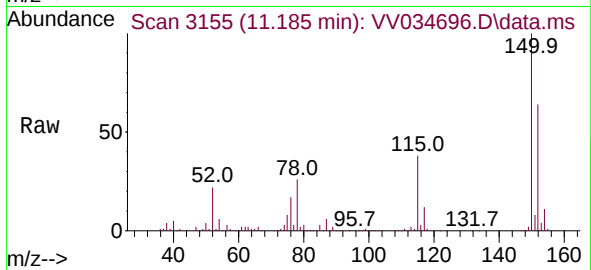

Tgt Ion:	75	Resp:	20012
Ion Ratio	Lower	Upper	
75	100		
77	36.4	25.9	38.9
110	3.4	33.1	49.7#

