

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034723.D
 Acq On : 19 Mar 2024 10:25
 Operator : SY/MD
 Sample : P1766-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 20 01:21:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	347390	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	324823	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	147983	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	150150	49.859	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	99.720%	
7) Chloroethane-d5	1.532	69	118868	50.665	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	101.320%	
11) 1,1-Dichloroethene-d2	2.060	65	66729	48.995	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	98.000%	
21) 2-Butanone-d5	3.790	46	173178	85.991	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	85.990%	
24) Chloroform-d	4.246	84	253297	47.570	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.140%	
26) 1,2-Dichloroethane-d4	4.941	65	170105	48.887	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.780%	
32) Benzene-d6	4.957	84	497456	50.744	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.480%	
36) 1,2-Dichloropropane-d6	5.986	67	152076	50.832	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	101.660%	
41) Toluene-d8	7.240	98	440222	49.622	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	99.240%	
43) trans-1,3-Dichloroprop...	7.551	79	68525	45.611	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.220%	
47) 2-Hexanone-d5	8.024	63	108831	72.848	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	72.850%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	192342	48.854	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	97.700%	
66) 1,2-Dichlorobenzene-d4	11.558	152	159093	52.596	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	105.200%	
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.185	75	17751	6.284	ug/L	# 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034723.D
Acq On : 19 Mar 2024 10:25
Operator : SY/MD
Sample : P1766-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 20 01:21:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

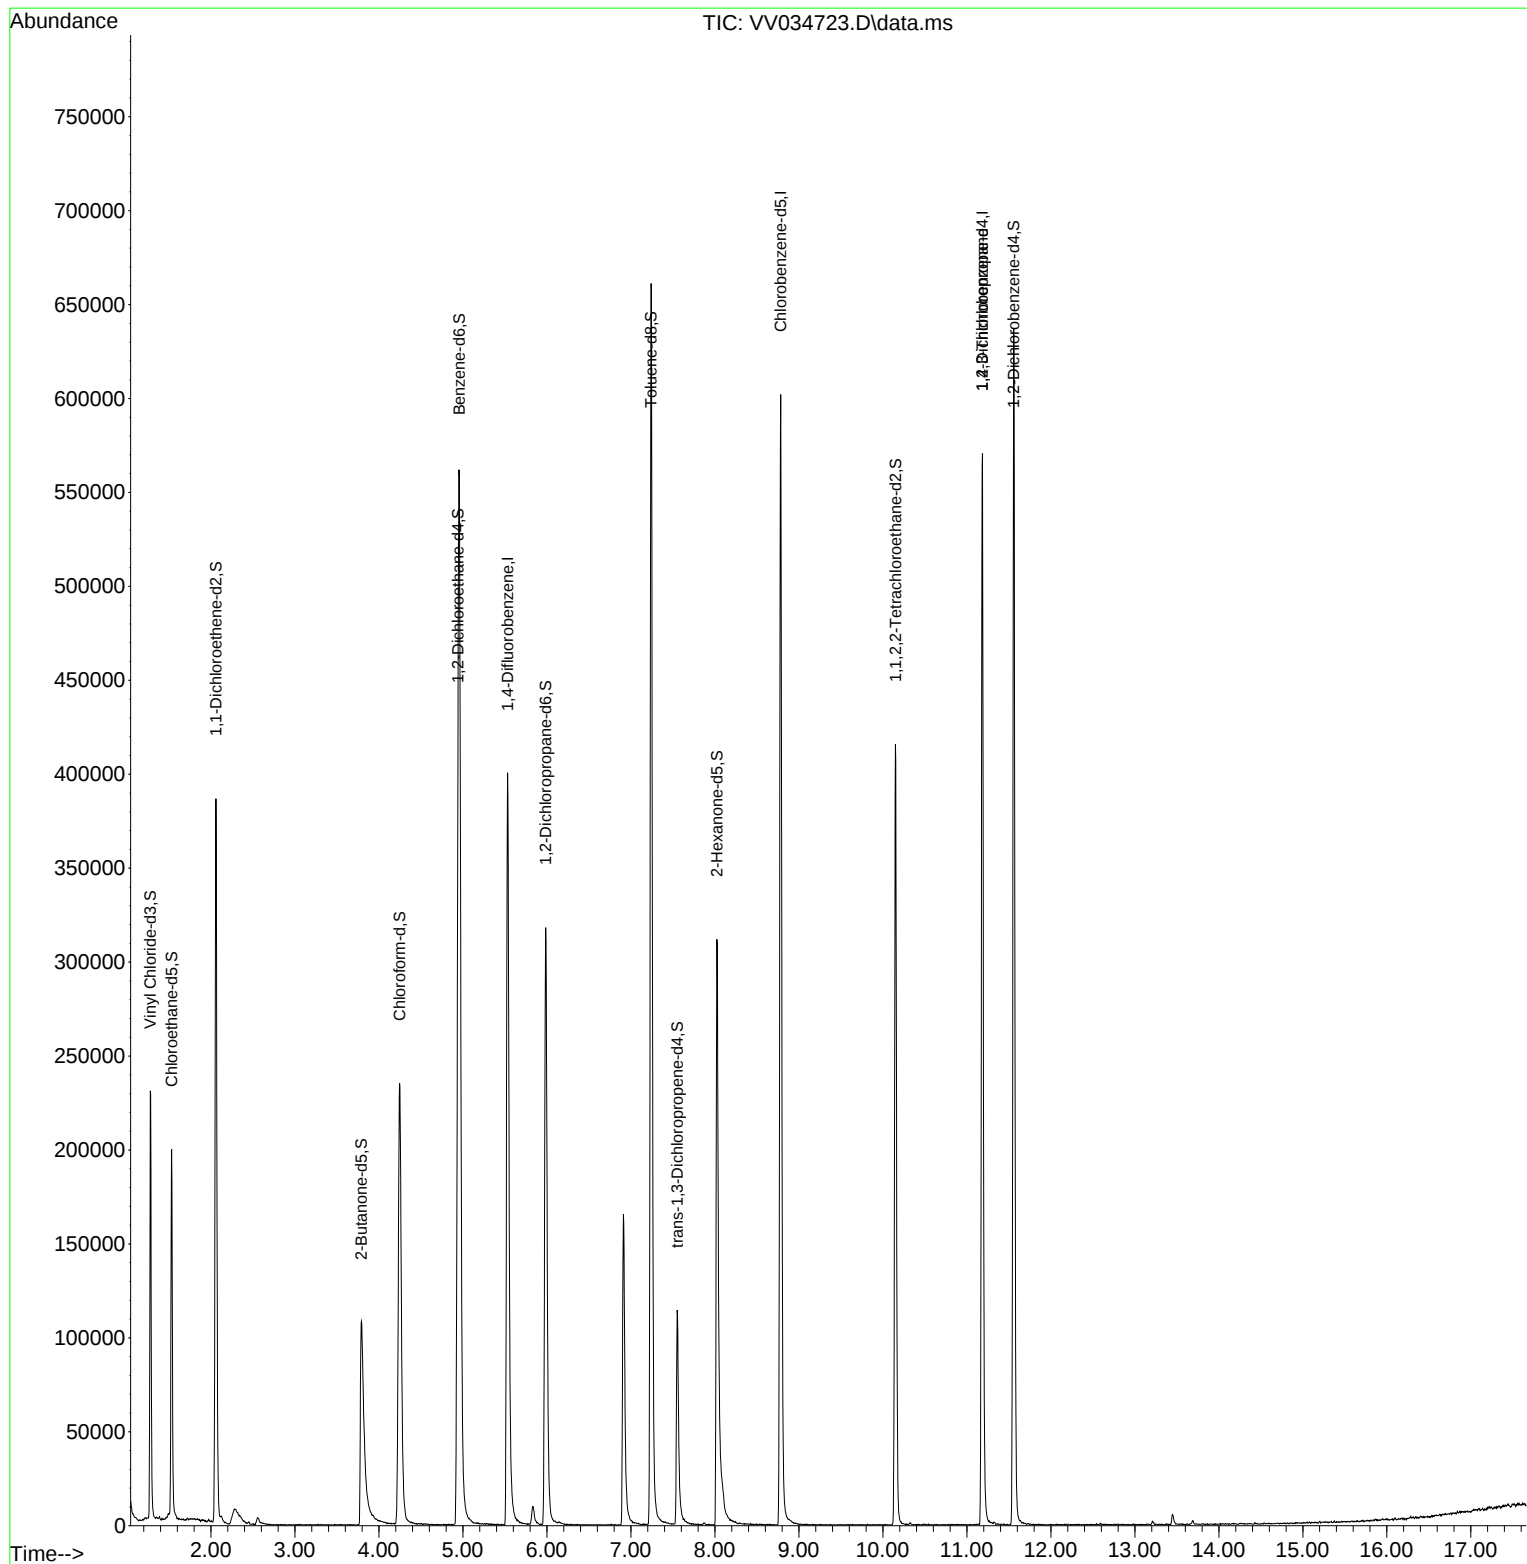

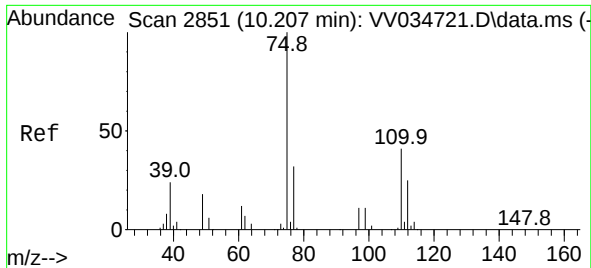

#61
 1,2,3-Trichloropropane
 Concen: 6.284 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.978 min
 Lab File: VV034723.D
 Acq: 19 Mar 2024 10:25

Instrument :
 MSVOA_V
 ClientSampleId :

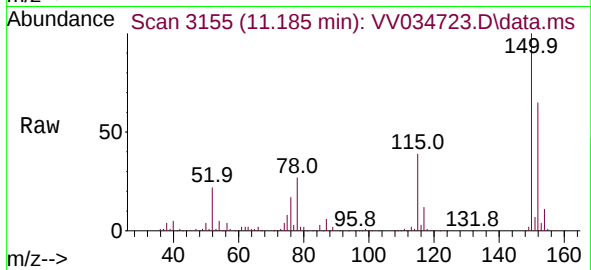

Tgt Ion:	75	Resp:	17751
Ion	Ratio	Lower	Upper
75	100		
77	34.6	25.9	38.9
110	3.0	33.1	49.7#

