

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034725.D
 Acq On : 19 Mar 2024 11:13
 Operator : SY/MD
 Sample : P1766-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 20 01:21:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	332328	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	318181	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	147593	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	149297	51.822	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 103.640%		
7) Chloroethane-d5	1.532	69	119415	53.205	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 106.400%		
11) 1,1-Dichloroethene-d2	2.060	65	67311	51.662	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 103.320%		
21) 2-Butanone-d5	3.789	46	189926	98.581	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 98.580%		
24) Chloroform-d	4.246	84	258925	50.831	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 101.660%		
26) 1,2-Dichloroethane-d4	4.937	65	182467	54.817	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 109.640%		
32) Benzene-d6	4.957	84	510472	53.159	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 106.320%		
36) 1,2-Dichloropropane-d6	5.986	67	161169	54.996	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 110.000%		
41) Toluene-d8	7.243	98	452336	52.052	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 104.100%		
43) trans-1,3-Dichloroprop...	7.551	79	75034	50.986	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 101.980%		
47) 2-Hexanone-d5	8.024	63	119349	81.556	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 81.560%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	207024	53.680	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 107.360%		
66) 1,2-Dichlorobenzene-d4	11.558	152	167926	55.663	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 111.320%		
Target Compounds			Qvalue			
61) 1,2,3-Trichloropropane	11.185	75	17735	6.295	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034725.D
Acq On : 19 Mar 2024 11:13
Operator : SY/MD
Sample : P1766-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 20 01:21:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

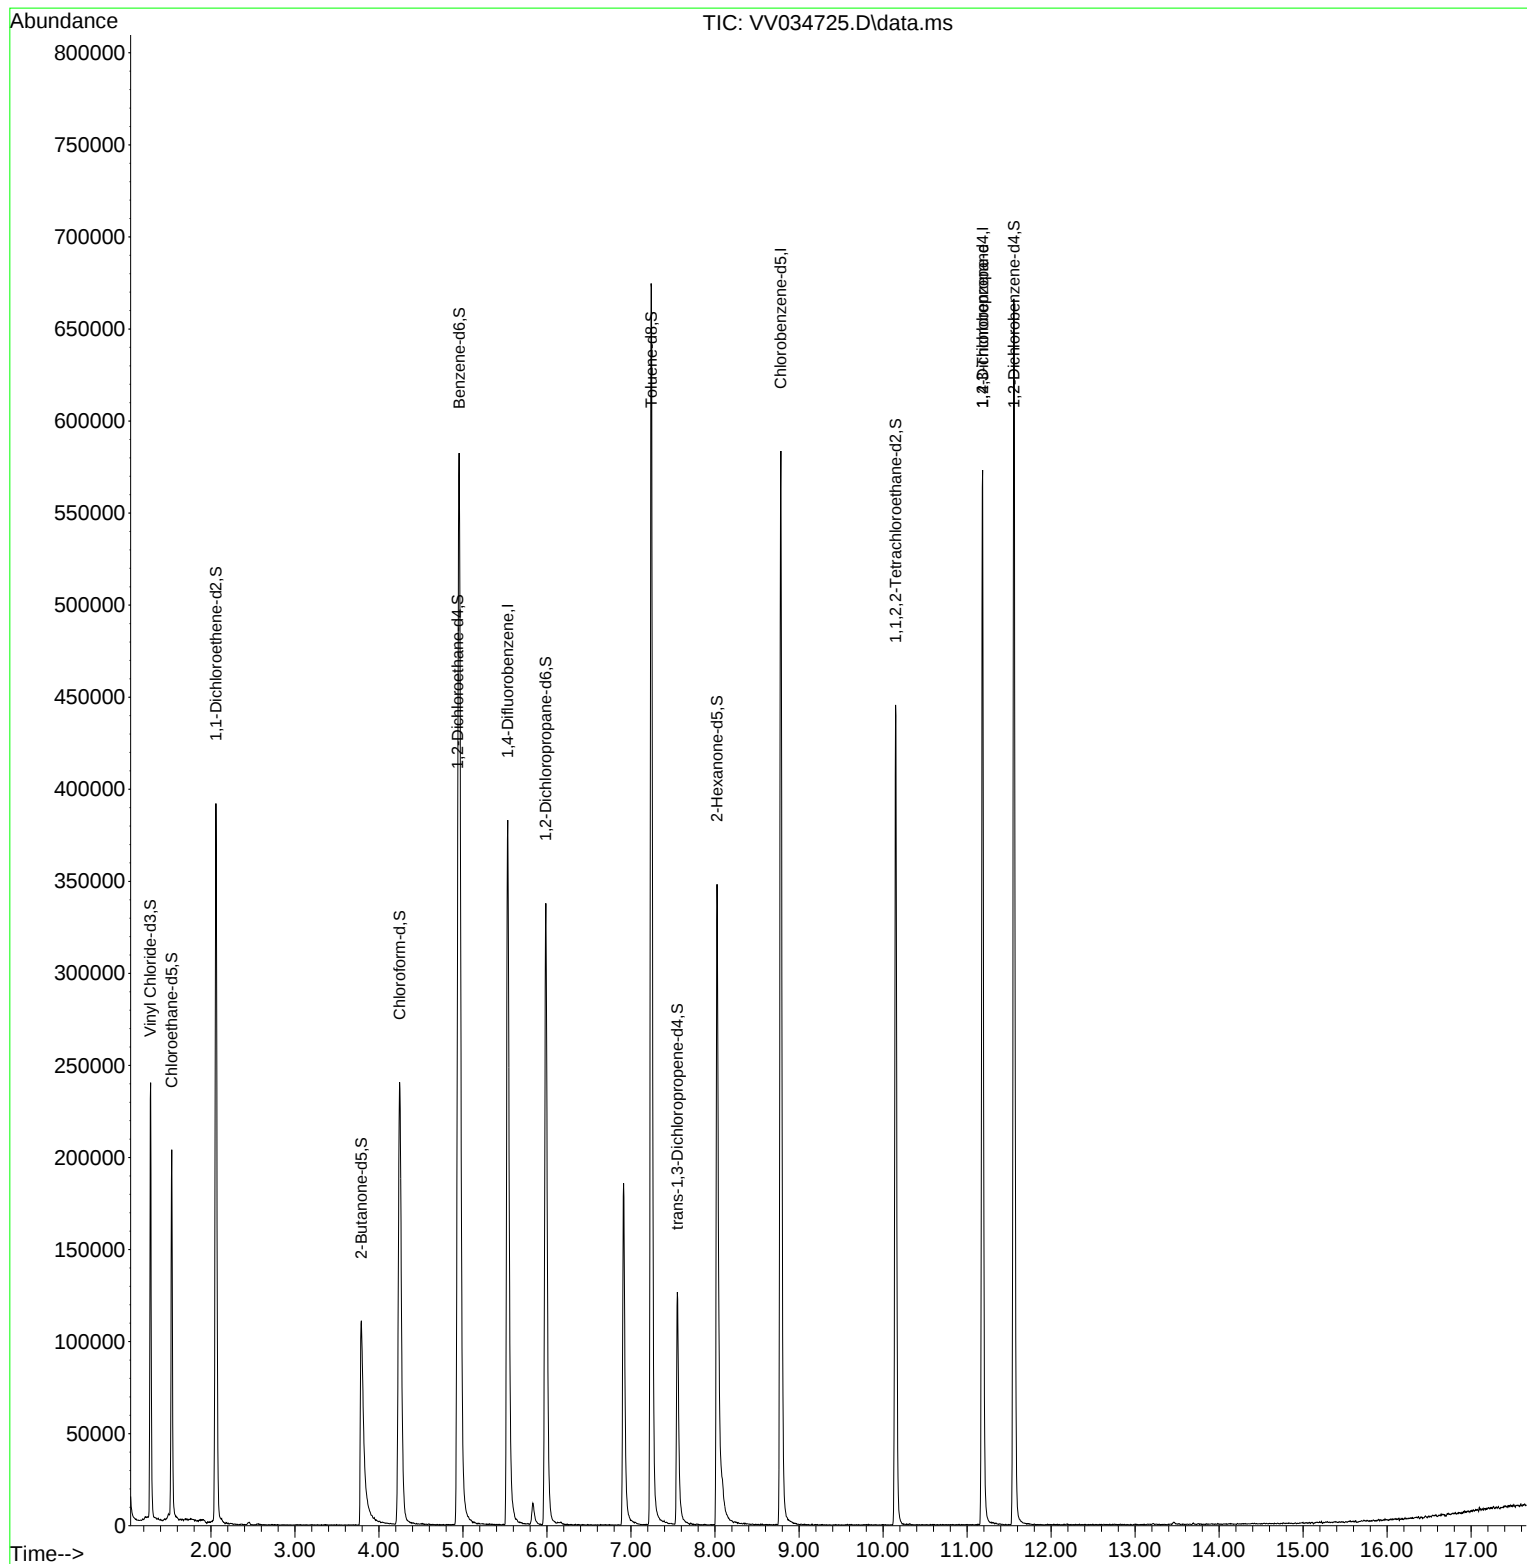

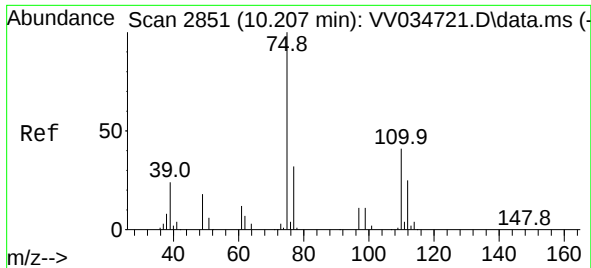

#61
 1,2,3-Trichloropropane
 Concen: 6.295 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.978 min
 Lab File: VV034725.D
 Acq: 19 Mar 2024 11:13

Instrument :
 MSVOA_V
 ClientSampleId :

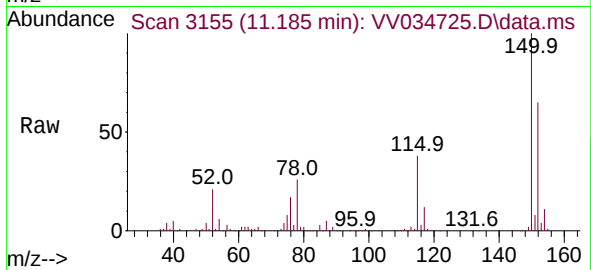

Tgt Ion: 75	Resp:	17735
Ion Ratio	Lower	Upper
75	100	
77	33.5	25.9 38.9
110	1.5	33.1 49.7#

