

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034735.D
 Acq On : 19 Mar 2024 15:10
 Operator : SY/MD
 Sample : P1752-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 20 01:24:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	389277	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	364796	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	171362	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	142223	42.145	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.280%
7) Chloroethane-d5	1.532	69	113720	43.255	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.500%
11) 1,1-Dichloroethene-d2	2.060	65	62602	41.019	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.040%
21) 2-Butanone-d5	3.790	46	184818	81.896	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.900%
24) Chloroform-d	4.246	84	250156	41.925	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.860%
26) 1,2-Dichloroethane-d4	4.941	65	167898	43.061	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.120%
32) Benzene-d6	4.960	84	492275	44.713	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.420%
36) 1,2-Dichloropropane-d6	5.986	67	151589	45.117	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.240%
41) Toluene-d8	7.243	98	438670	44.029	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.060%
43) trans-1,3-Dichloroprop...	7.551	79	74407	44.100	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.200%
47) 2-Hexanone-d5	8.024	63	113842	67.852	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.850%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	195365	44.184	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.360%
66) 1,2-Dichlorobenzene-d4	11.558	152	160932	45.945	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.900%
Target Compounds						
61) 1,2,3-Trichloropropane	11.185	75	19867	6.074	ug/L	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034735.D
Acq On : 19 Mar 2024 15:10
Operator : SY/MD
Sample : P1752-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 20 01:24:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

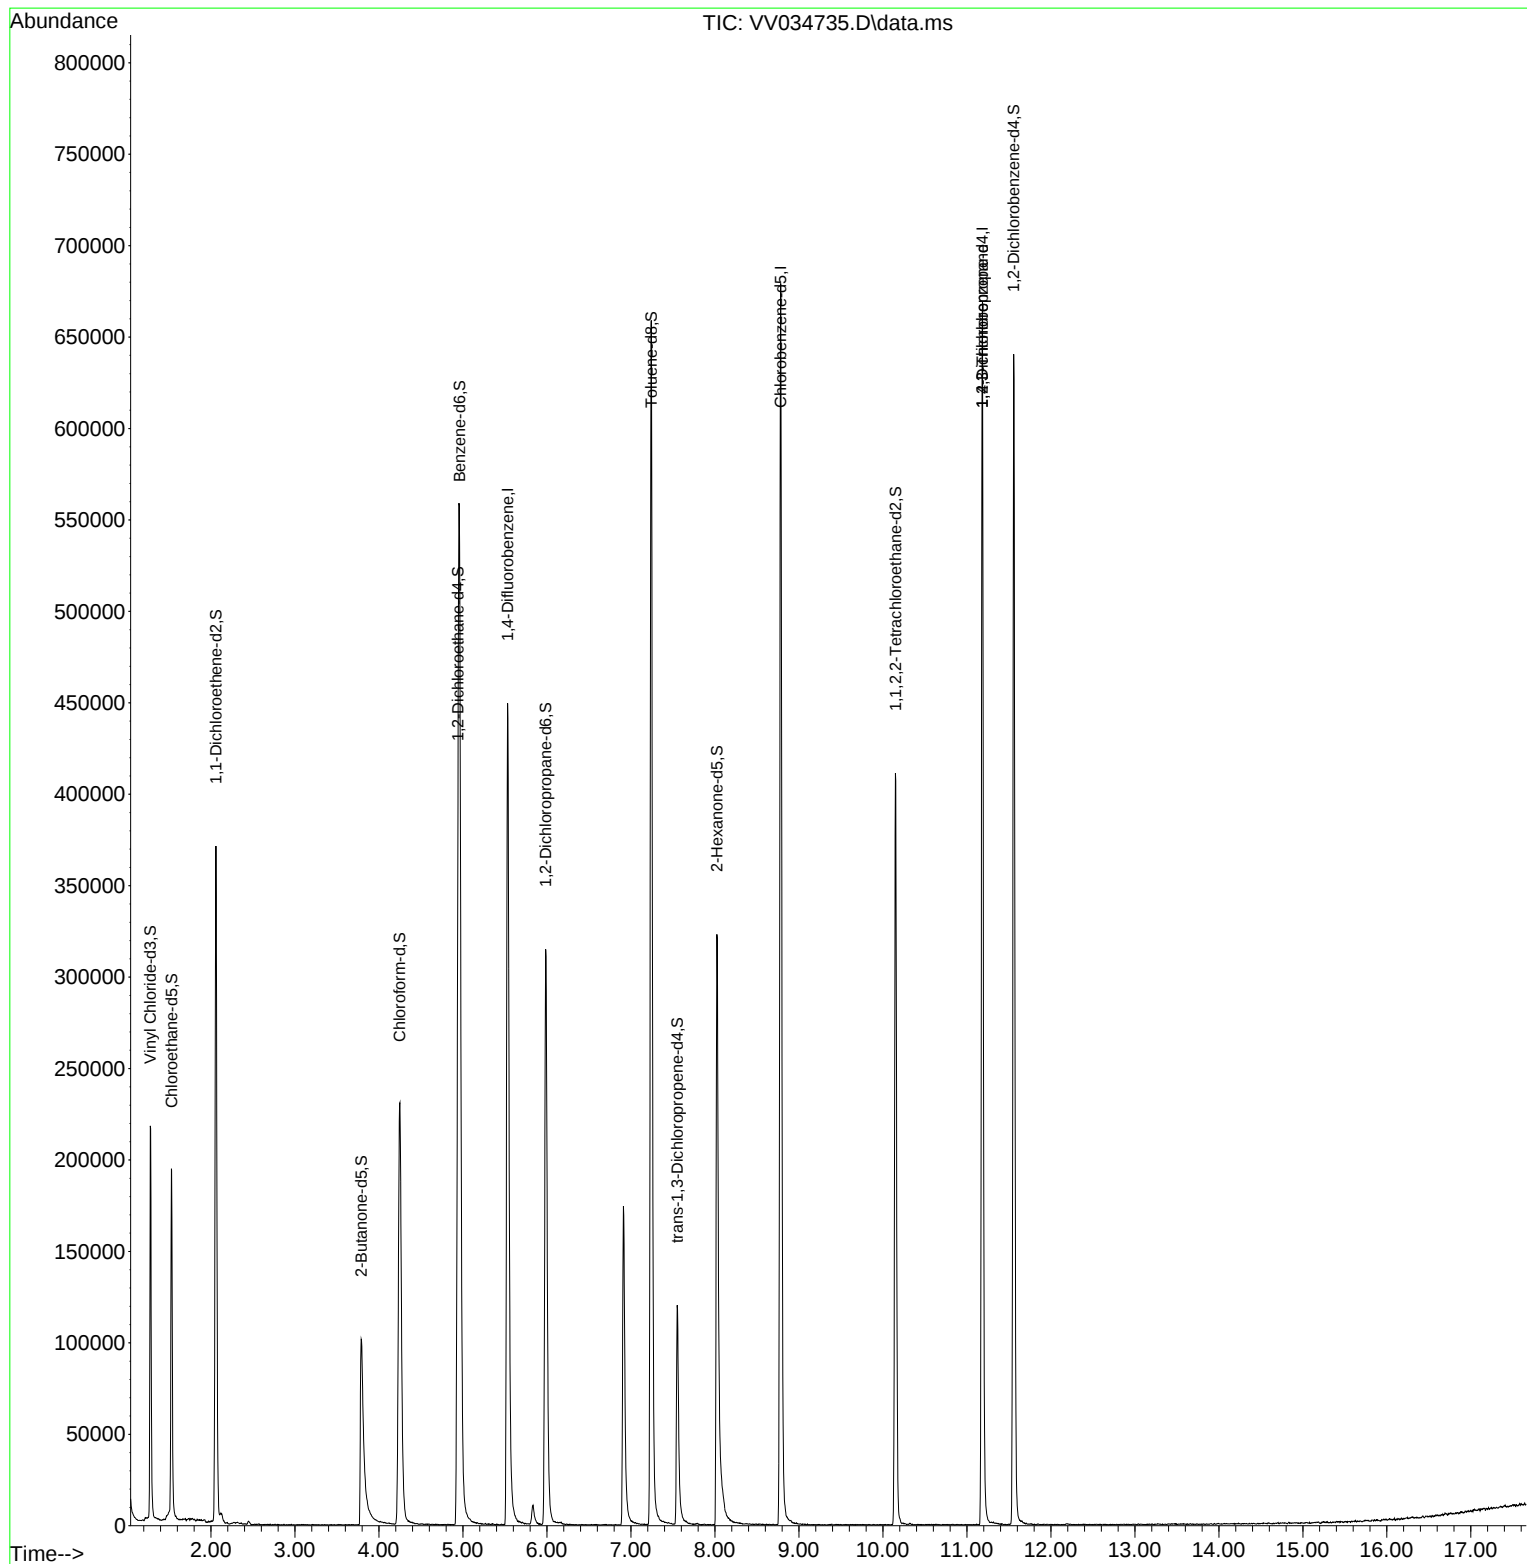

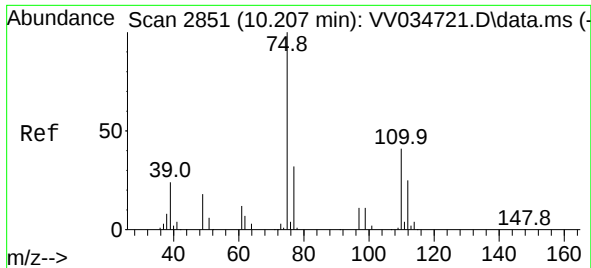

#61
 1,2,3-Trichloropropane
 Concen: 6.074 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.978 min
 Lab File: VV034735.D
 Acq: 19 Mar 2024 15:10

Instrument :
 MSVOA_V
 ClientSampleId :

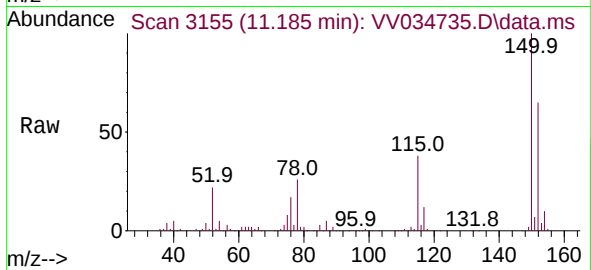

Tgt Ion: 75 Resp: 19867
 Ion Ratio Lower Upper
 75 100
 77 34.8 25.9 38.9
 110 3.0 33.1 49.7#

