

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034737.D
 Acq On : 19 Mar 2024 15:58
 Operator : SY/MD
 Sample : P1756-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 20 01:24:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	256814	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	243885	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	108495	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	101006	45.369	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.740%		
7) Chloroethane-d5	1.526	69	82707	47.685	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.360%		
11) 1,1-Dichloroethene-d2	2.056	65	45599	45.289	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.580%		
21) 2-Butanone-d5	3.793	46	173359	116.441	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	116.440%		
24) Chloroform-d	4.249	84	194653	49.450	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.900%		
26) 1,2-Dichloroethane-d4	4.940	65	136470	53.053	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.100%		
32) Benzene-d6	4.957	84	379420	51.548	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.100%		
36) 1,2-Dichloropropane-d6	5.989	67	119802	53.333	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	106.660%		
41) Toluene-d8	7.243	98	325331	48.842	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.680%		
43) trans-1,3-Dichloroprop...	7.555	79	58135	51.537	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	103.080%		
47) 2-Hexanone-d5	8.027	63	103955	92.677	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.680%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	160965	54.452	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	108.900%		
66) 1,2-Dichlorobenzene-d4	11.561	152	118163	53.282	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.560%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	4020	1.252	ug/L #	82
61) 1,2,3-Trichloropropane	11.181	75	12533	6.052	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034737.D
Acq On : 19 Mar 2024 15:58
Operator : SY/MD
Sample : P1756-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 20 01:24:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

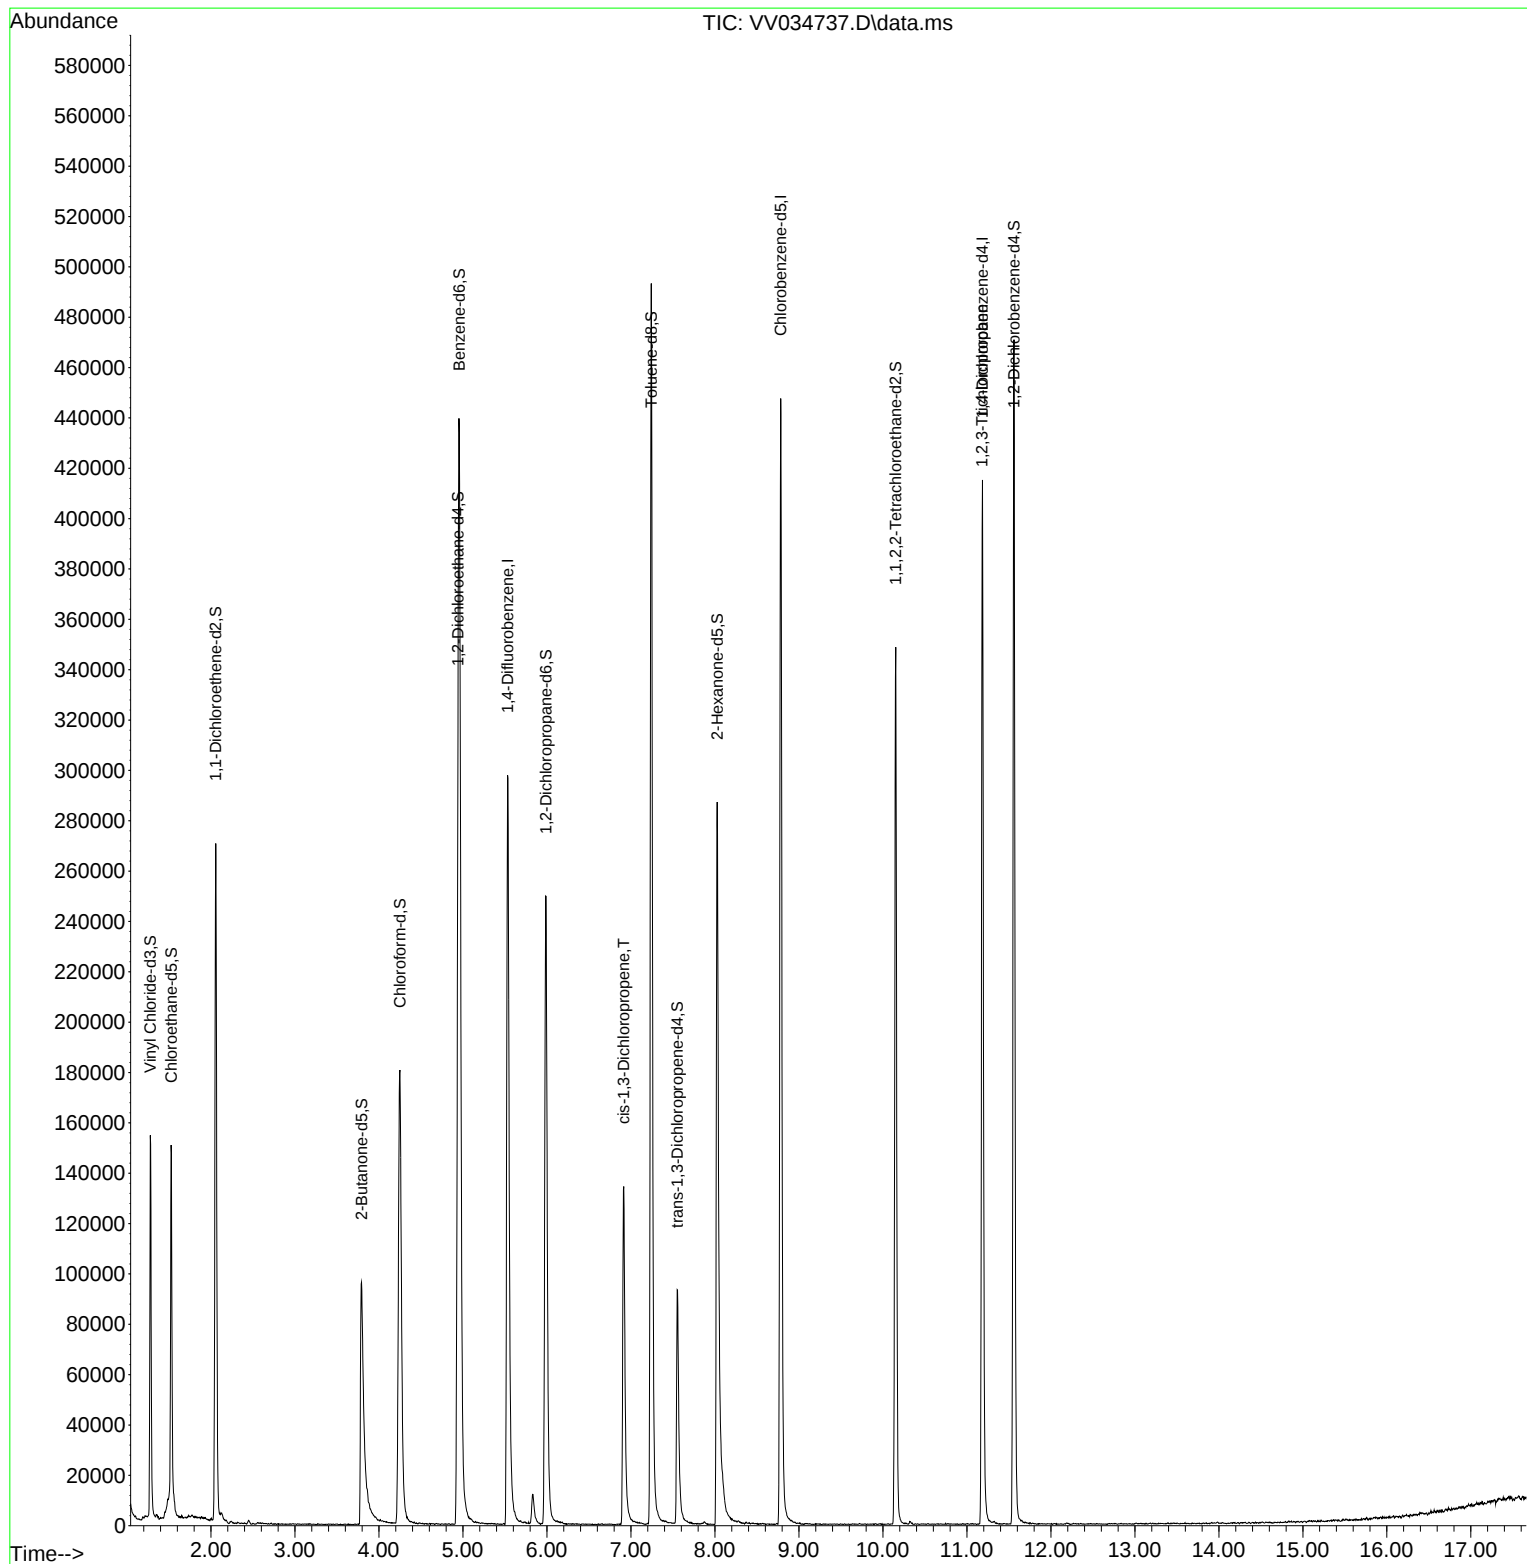

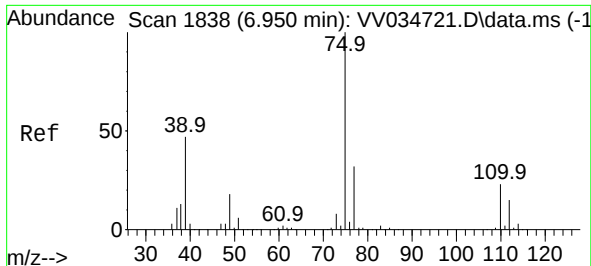

#39

cis-1,3-Dichloropropene

Concen: 1.252 ug/L

RT: 6.915 min Scan# 11

Delta R.T. -0.035 min

Lab File: VV034737.D

Acq: 19 Mar 2024 15:58

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 4020

Ion Ratio Lower Upper

75 100

77 39.6 20.9 38.9#

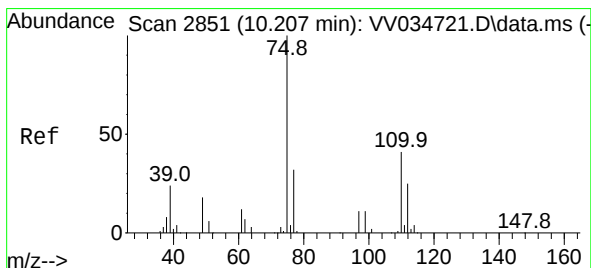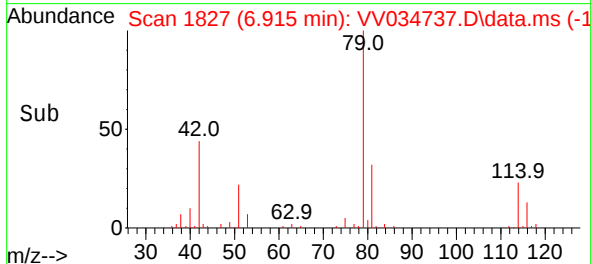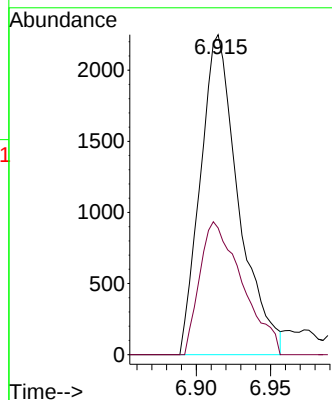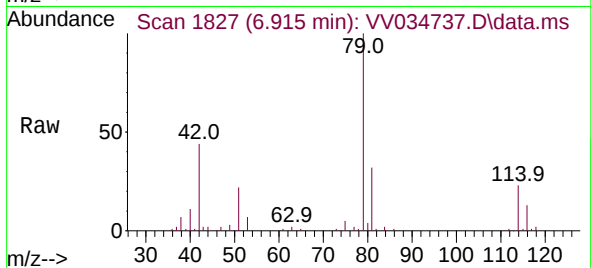

#61

1,2,3-Trichloropropane

Concen: 6.052 ug/L

RT: 11.181 min Scan# 3154

Delta R.T. 0.974 min

Lab File: VV034737.D

Acq: 19 Mar 2024 15:58

Tgt Ion: 75 Resp: 12533

Ion Ratio Lower Upper

75 100

77 32.3 25.9 38.9

110 2.7 33.1 49.7#

