

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034738.D
 Acq On : 19 Mar 2024 16:21
 Operator : SY/MD
 Sample : P1756-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 20 01:25:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	300803	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	281686	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	130195	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	126976	48.694	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	97.380%		
7) Chloroethane-d5	1.529	69	104005	51.195	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	102.400%		
11) 1,1-Dichloroethene-d2	2.060	65	56825	48.185	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.380%		
21) 2-Butanone-d5	3.789	46	176968	101.482	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.480%		
24) Chloroform-d	4.246	84	229484	49.773	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.540%		
26) 1,2-Dichloroethane-d4	4.941	65	154148	51.162	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.320%		
32) Benzene-d6	4.960	84	450442	52.985	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.960%		
36) 1,2-Dichloropropane-d6	5.989	67	137529	53.009	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	106.020%		
41) Toluene-d8	7.243	98	394483	51.276	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.560%		
43) trans-1,3-Dichloroprop...	7.551	79	65504	50.277	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	100.560%		
47) 2-Hexanone-d5	8.024	63	105253	81.242	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	81.240%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	177691	52.044	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.080%		
66) 1,2-Dichlorobenzene-d4	11.561	152	149103	56.028	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	112.060%		
Target Compounds						Qvalue
13) Acetone	2.118	43	302446	144.271	ug/L	99
37) 1,2-Dichloropropane	5.986	63	15938	6.962	ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034738.D
Acq On : 19 Mar 2024 16:21
Operator : SY/MD
Sample : P1756-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 20 01:25:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

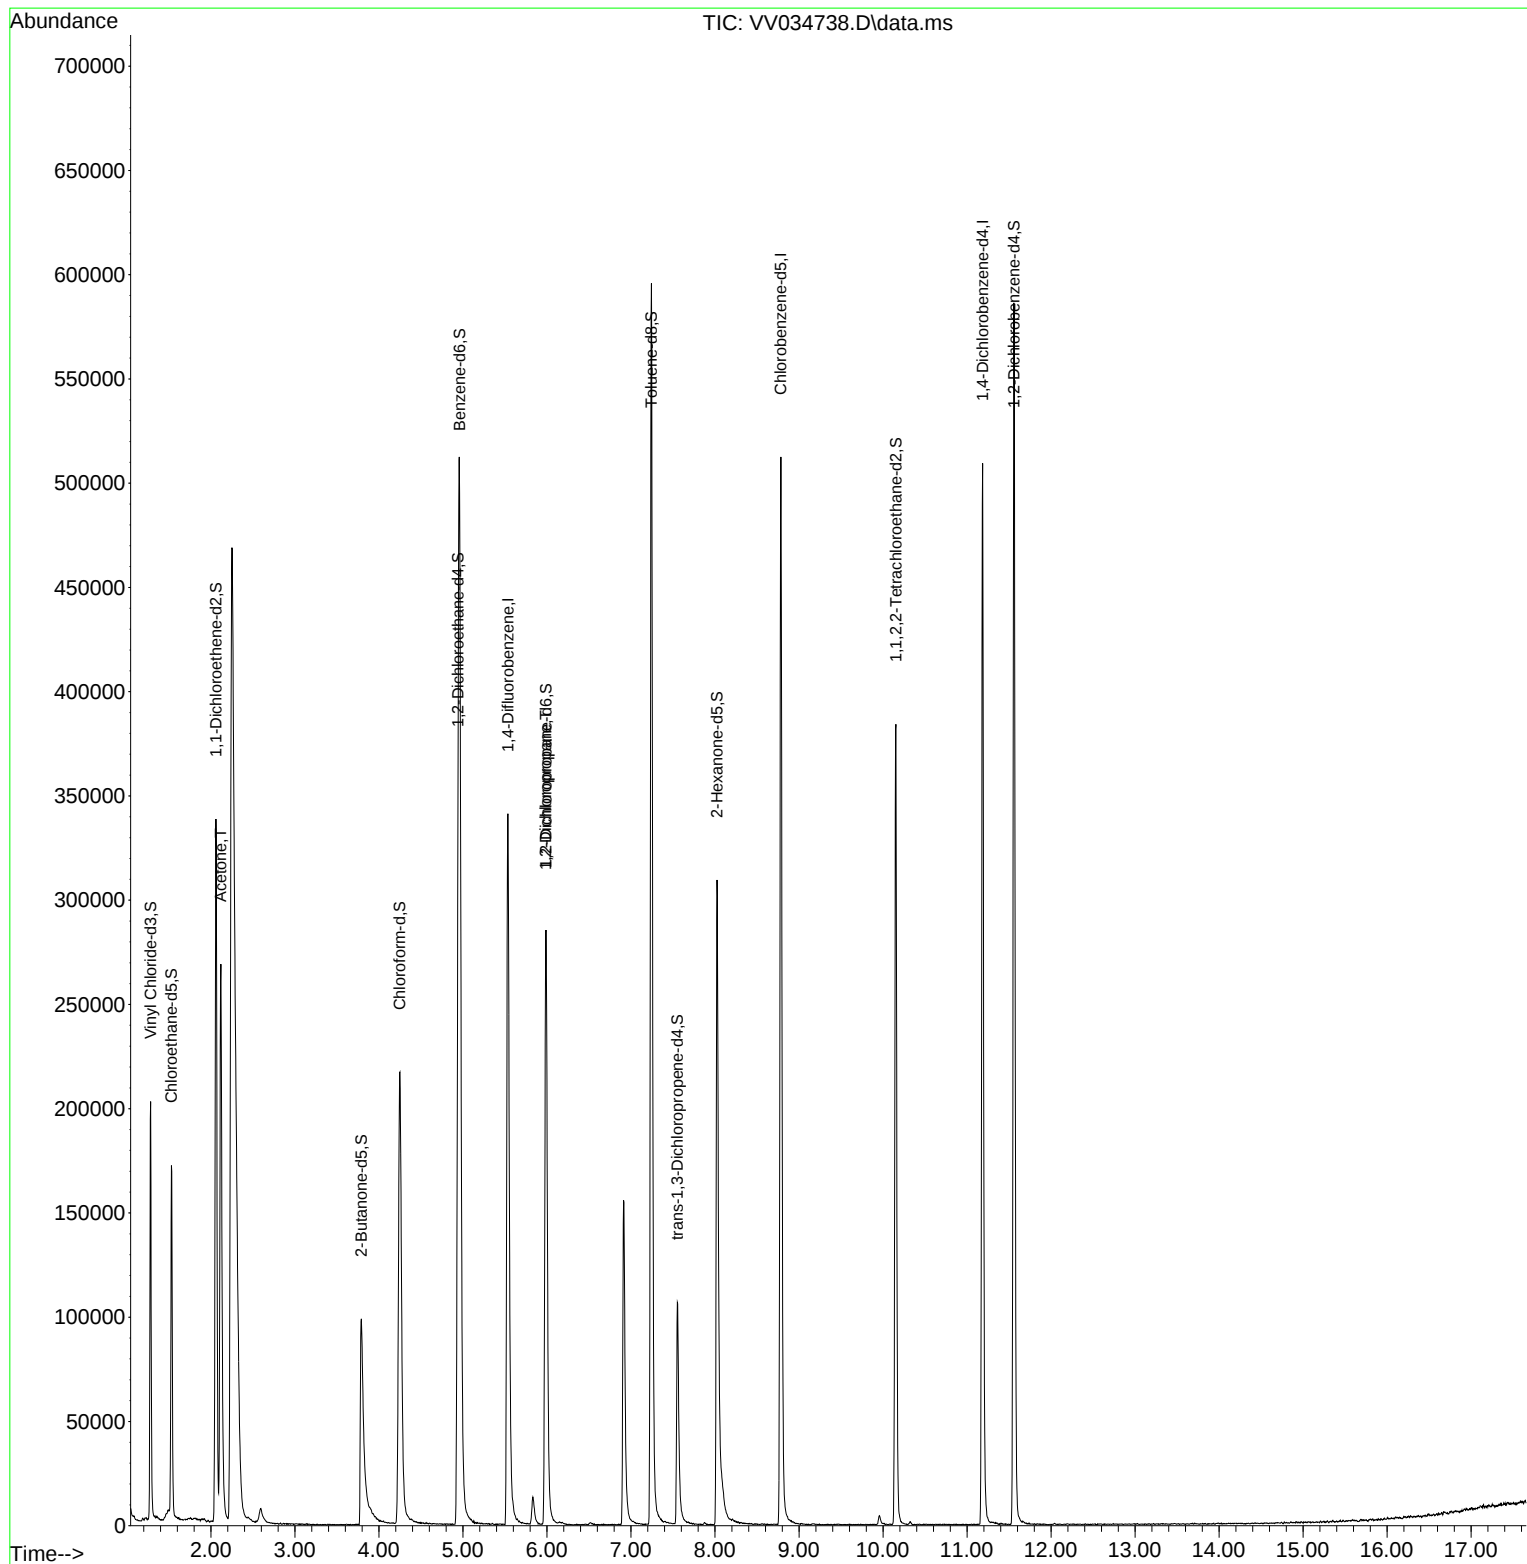

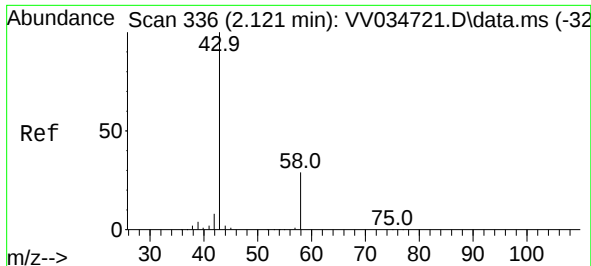

#13

Acetone

Concen: 144.271 ug/L

RT: 2.118 min Scan# 30

Delta R.T. -0.003 min

Lab File: VV034738.D

Acq: 19 Mar 2024 16:21

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 302446

Ion Ratio Lower Upper

43 100

58 28.3 0.0 57.2

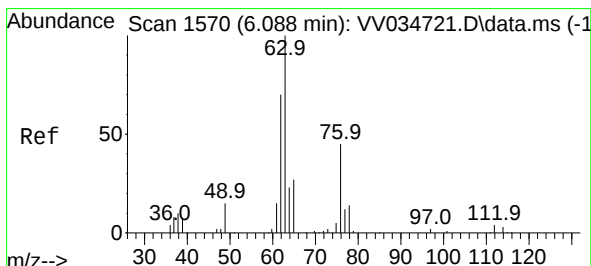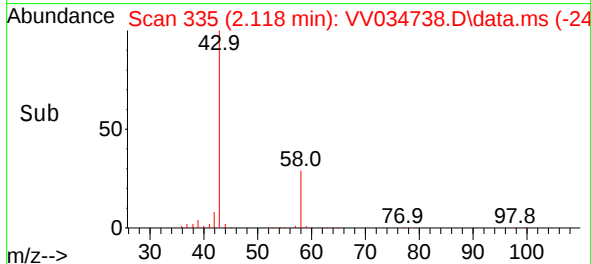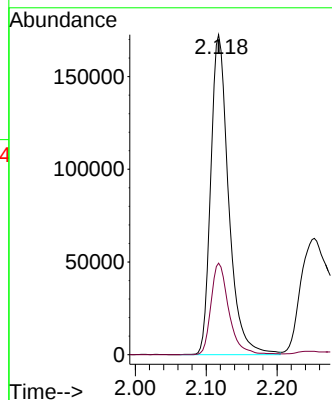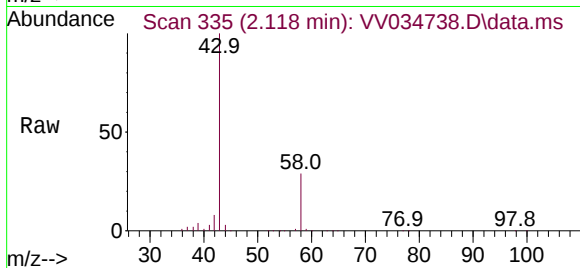

#37

1,2-Dichloropropane

Concen: 6.962 ug/L

RT: 5.986 min Scan# 1538

Delta R.T. -0.103 min

Lab File: VV034738.D

Acq: 19 Mar 2024 16:21

Tgt Ion: 63 Resp: 15938

Ion Ratio Lower Upper

63 100

112 0.0 3.5 5.3#

