

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034739.D
 Acq On : 19 Mar 2024 16:45
 Operator : SY/MD
 Sample : P1756-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 20 01:25:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	330875	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	308747	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	142824	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	134133	46.763	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	93.520%	
7) Chloroethane-d5	1.529	69	111981	50.111	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	100.220%	
11) 1,1-Dichloroethene-d2	2.060	65	60066	46.304	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.600%	
21) 2-Butanone-d5	3.790	46	179478	93.567	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	93.570%	
24) Chloroform-d	4.249	84	241012	47.523	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.040%	
26) 1,2-Dichloroethane-d4	4.941	65	161913	48.855	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.720%	
32) Benzene-d6	4.960	84	470274	50.469	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.940%	
36) 1,2-Dichloropropane-d6	5.989	67	143846	50.584	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	101.160%	
41) Toluene-d8	7.243	98	408087	48.395	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.780%	
43) trans-1,3-Dichloroprop...	7.555	79	68943	48.279	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.560%	
47) 2-Hexanone-d5	8.024	63	108110	76.133	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	76.130%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	184401	49.275	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.560%	
66) 1,2-Dichlorobenzene-d4	11.561	152	153837	52.695	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	105.400%	
Target Compounds						
61) 1,2,3-Trichloropropane	11.182	75	16150	5.924	ug/L	Qvalue # 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034739.D
Acq On : 19 Mar 2024 16:45
Operator : SY/MD
Sample : P1756-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 20 01:25:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

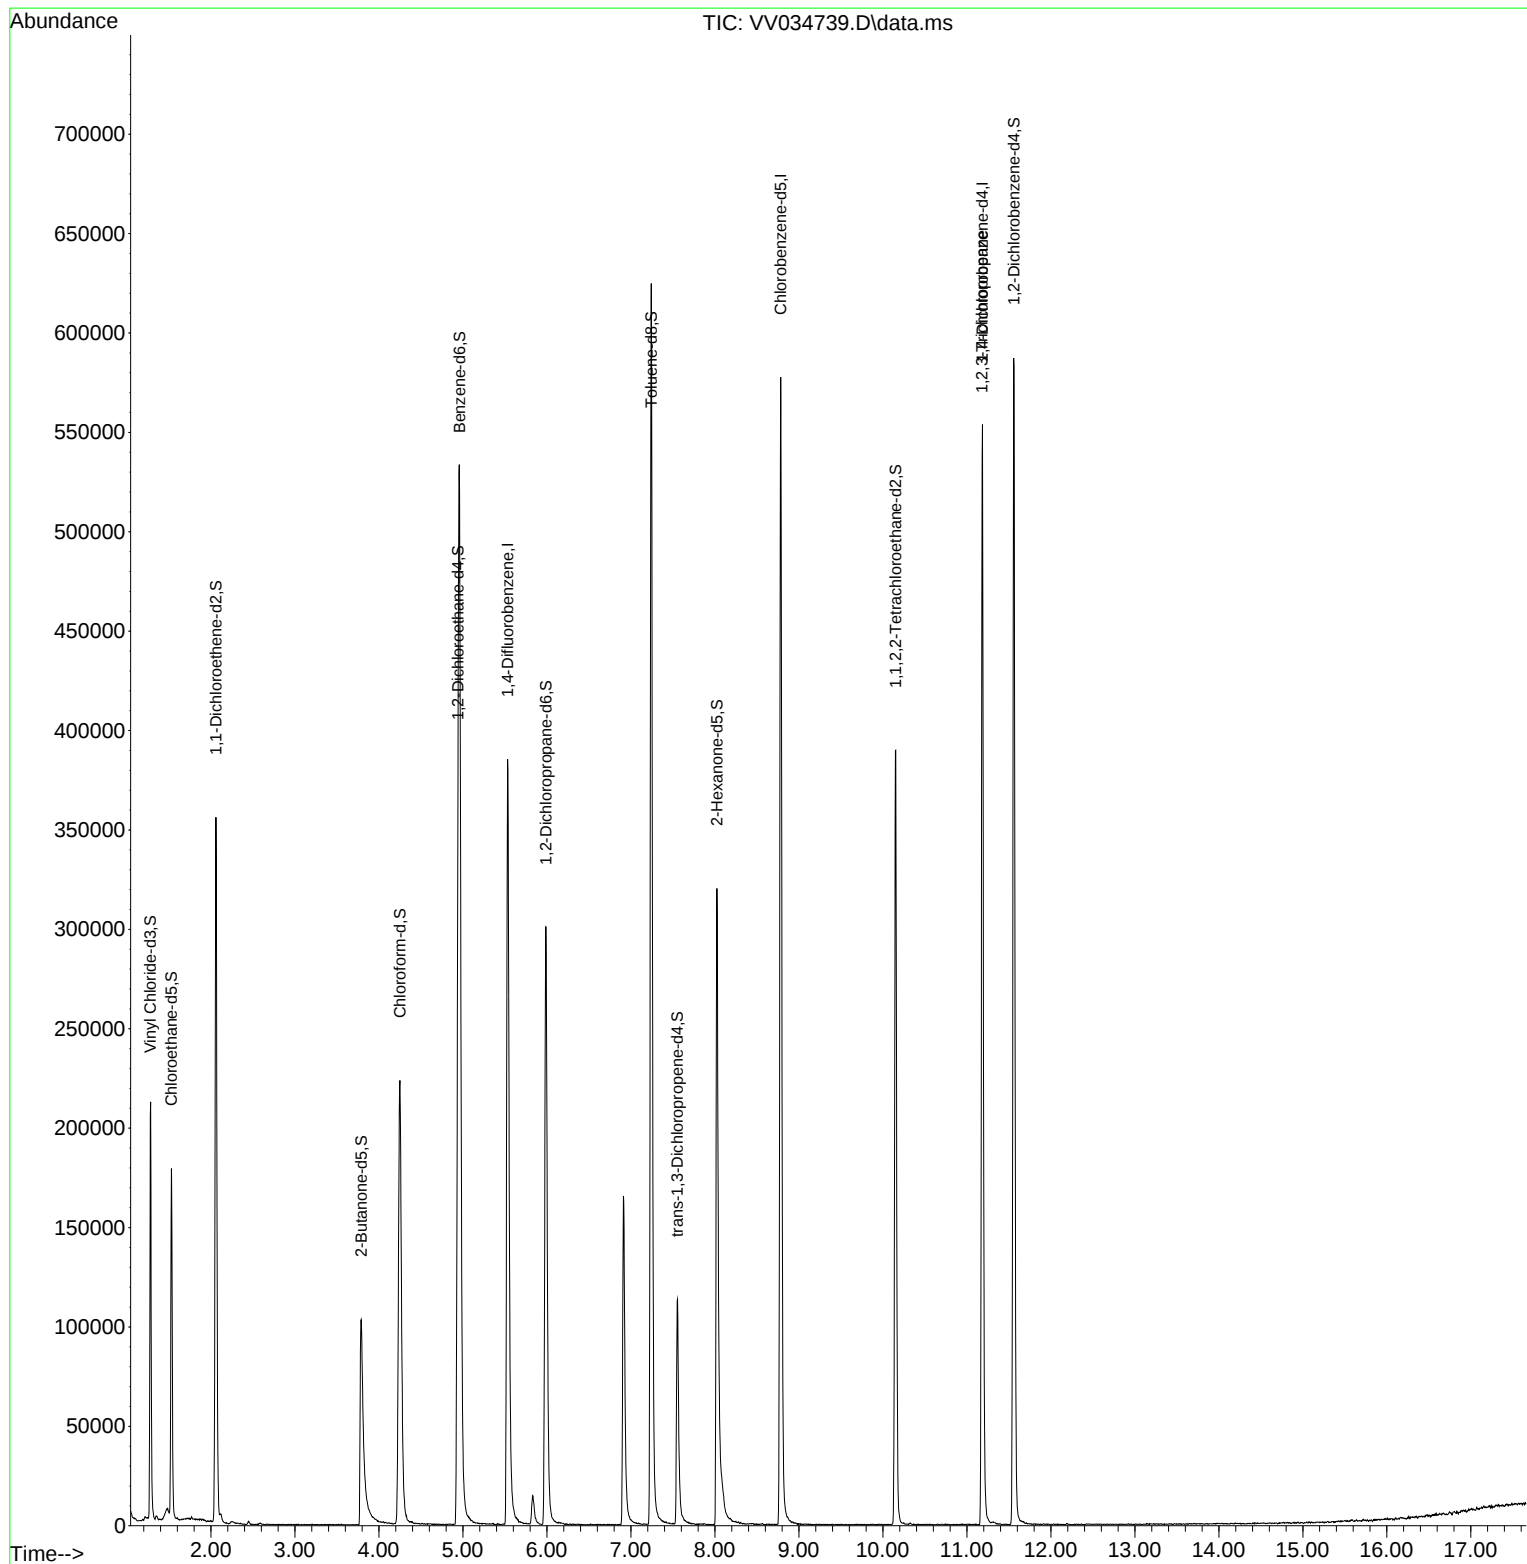

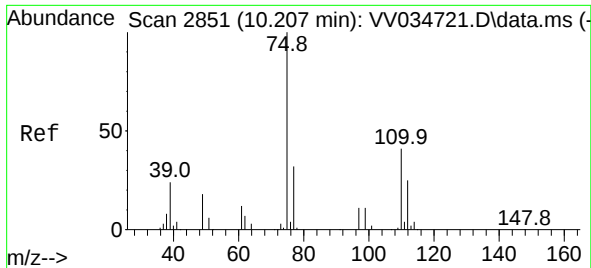

#61

1,2,3-Trichloropropane

Concen: 5.924 ug/L

RT: 11.182 min Scan# 31

Delta R.T. 0.974 min


Lab File: VV034739.D

Acq: 19 Mar 2024 16:45

Instrument :

MSVOA_V

ClientSampleId :

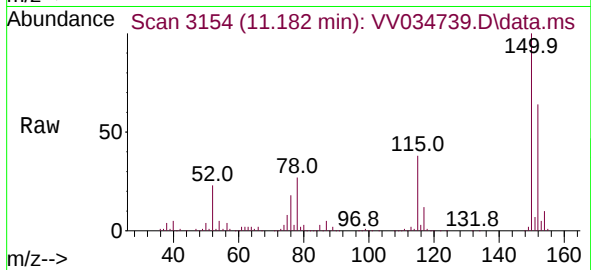

Tgt Ion: 75 Resp: 16150

Ion Ratio Lower Upper

75 100

77 36.7 25.9 38.9

110 2.5 33.1 49.7#

