

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034741.D
 Acq On : 19 Mar 2024 17:33
 Operator : SY/MD
 Sample : P1755-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 20 01:25:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	286384	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	273431	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	124843	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	125859	50.695	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.400%
7) Chloroethane-d5	1.529	69	103607	53.567	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.140%
11) 1,1-Dichloroethene-d2	2.060	65	55730	49.636	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.280%
21) 2-Butanone-d5	3.786	46	159935	96.332	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.330%
24) Chloroform-d	4.246	84	226564	51.614	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.220%
26) 1,2-Dichloroethane-d4	4.941	65	153839	53.631	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.260%
32) Benzene-d6	4.957	84	442674	53.643	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.280%
36) 1,2-Dichloropropane-d6	5.989	67	136374	54.151	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.300%
41) Toluene-d8	7.243	98	386472	51.751	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.500%
43) trans-1,3-Dichloroprop...	7.551	79	64266	50.816	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.640%
47) 2-Hexanone-d5	8.024	63	99974	79.497	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.500%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	175943	53.088	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	106.180%
66) 1,2-Dichlorobenzene-d4	11.561	152	142974	56.028	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.060%
Target Compounds						Qvalue
13) Acetone	2.114	43	122286	61.269	ug/L	99
39) cis-1,3-Dichloropropene	6.915	75	4387	1.219	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034741.D
Acq On : 19 Mar 2024 17:33
Operator : SY/MD
Sample : P1755-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 20 01:25:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

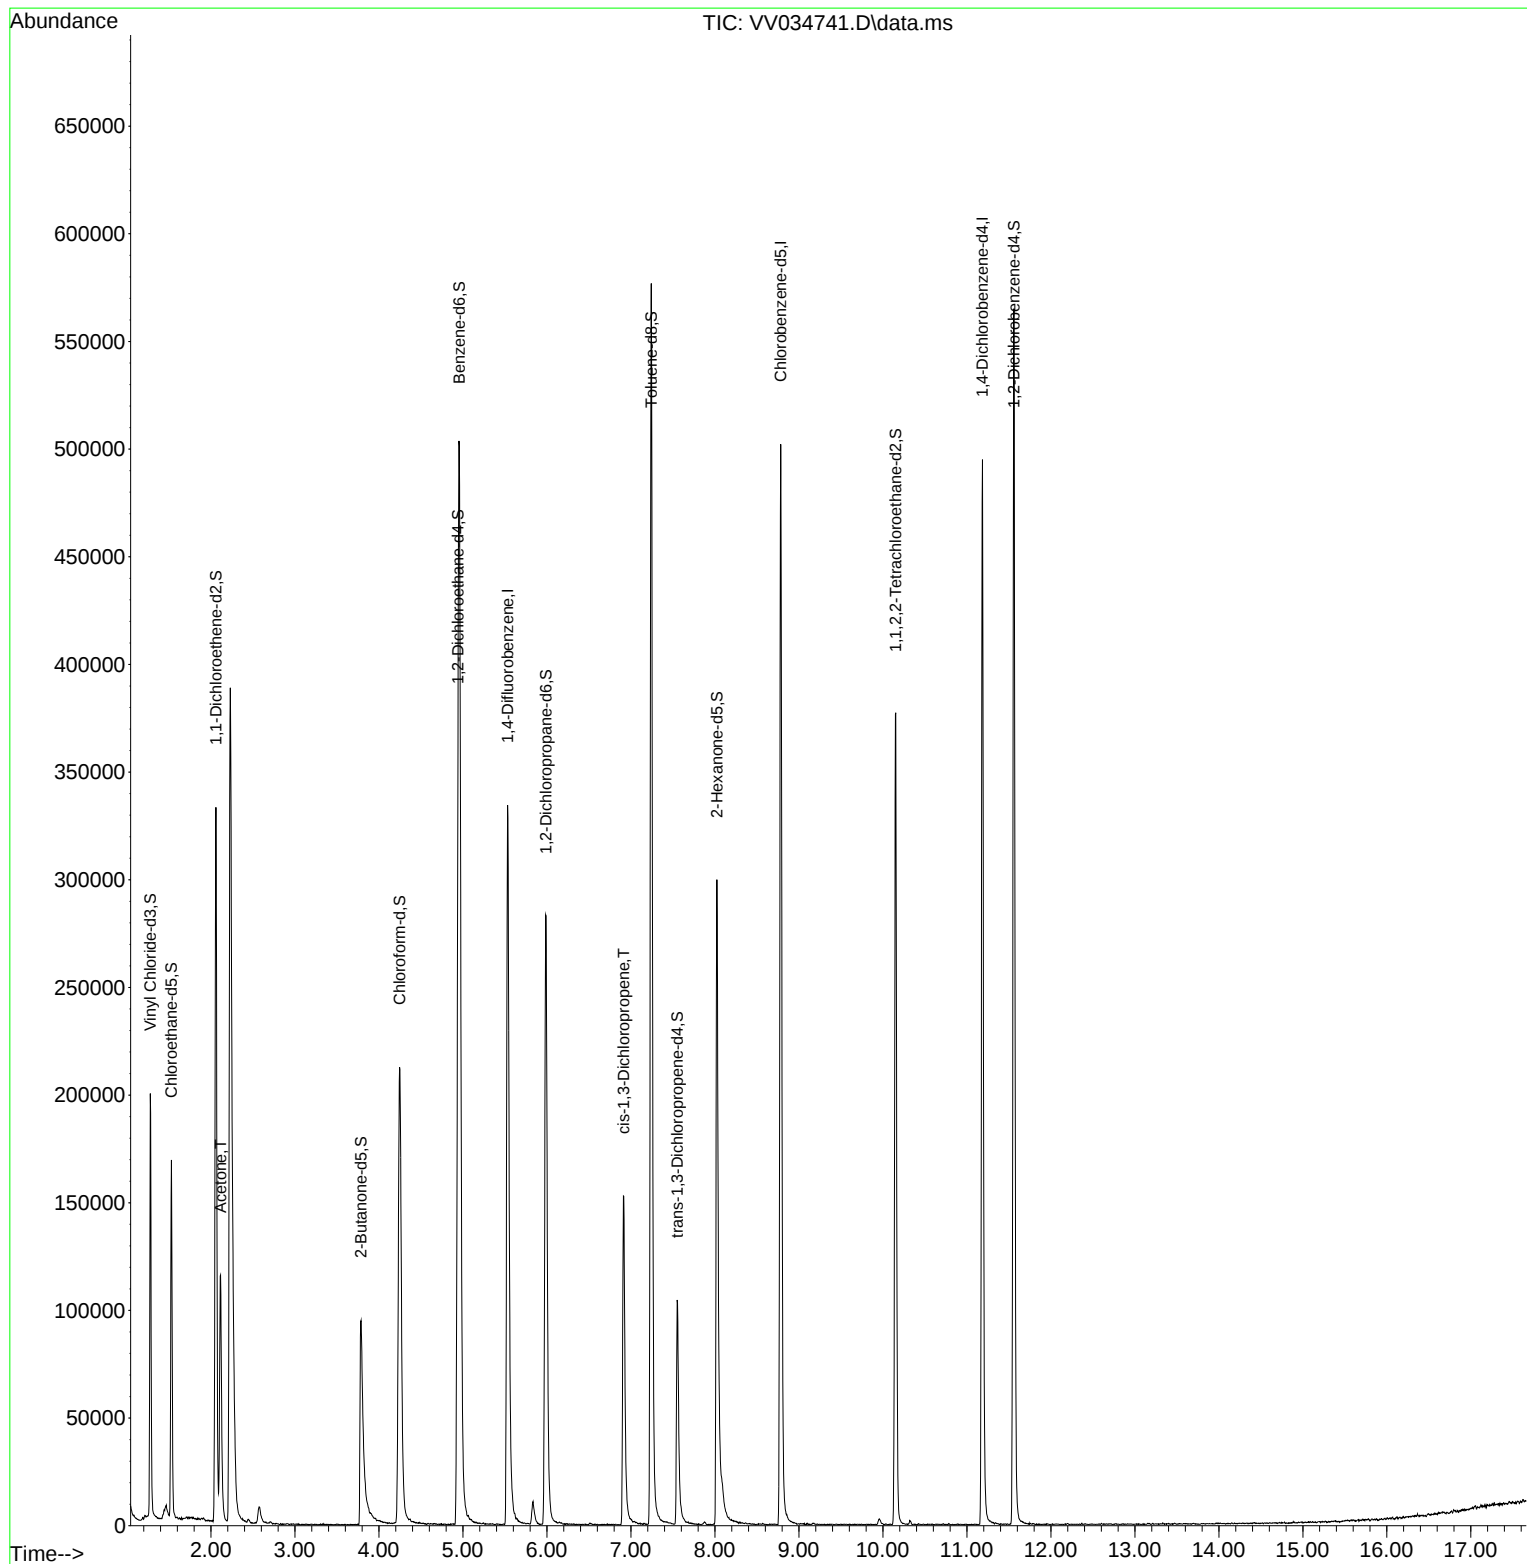

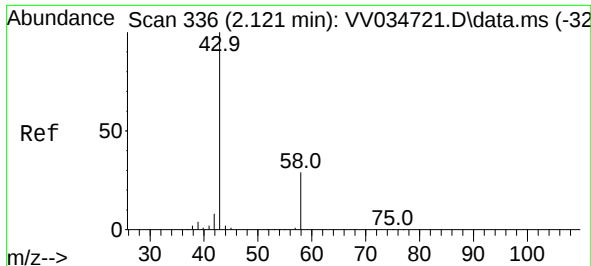

#13

Acetone

Concen: 61.269 ug/L

RT: 2.114 min Scan# 336

Delta R.T. -0.006 min

Lab File: VV034741.D

Acq: 19 Mar 2024 17:33

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 122286

Ion Ratio Lower Upper

43 100

58 29.1 0.0 57.2

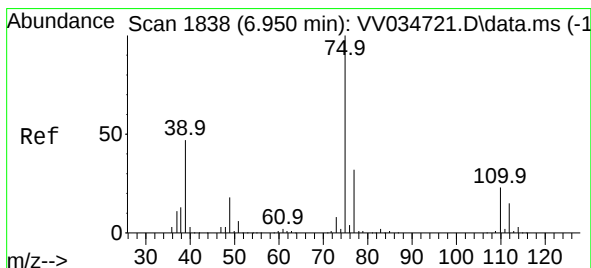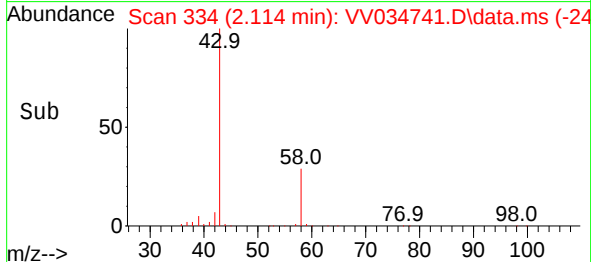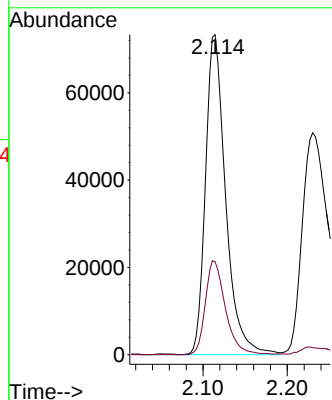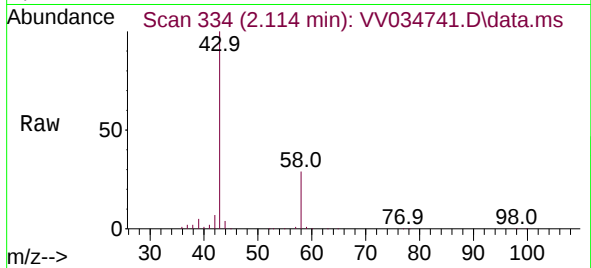

#39

cis-1,3-Dichloropropene

Concen: 1.219 ug/L

RT: 6.915 min Scan# 1827

Delta R.T. -0.035 min

Lab File: VV034741.D

Acq: 19 Mar 2024 17:33

Tgt Ion: 75 Resp: 4387

Ion Ratio Lower Upper

75 100

77 49.7 20.9 38.9#

