




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034728.D
 Acq On : 19 Mar 2024 12:24
 Operator : SY/MD
 Sample : P1751-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL18

Manual IntegrationsAPPROVED

Quant Time: Mar 20 01:22:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/20/2024
 Supervised By :Semsettin Yesilyurt 03/20/2024

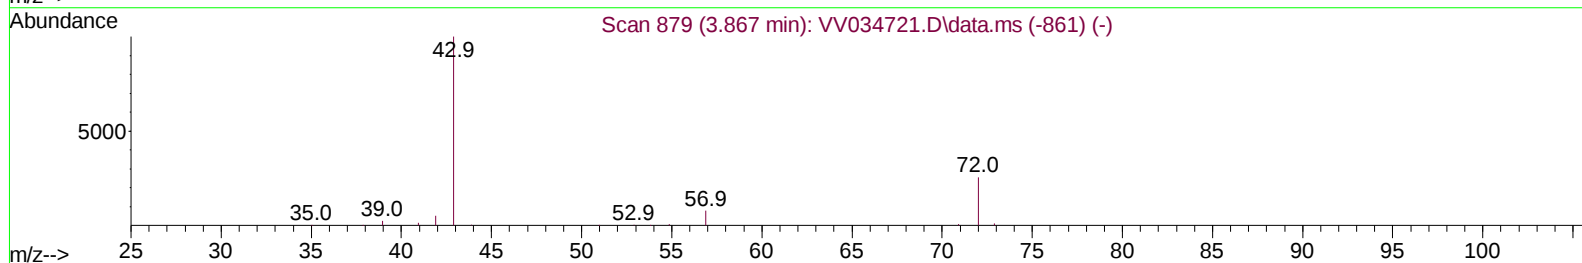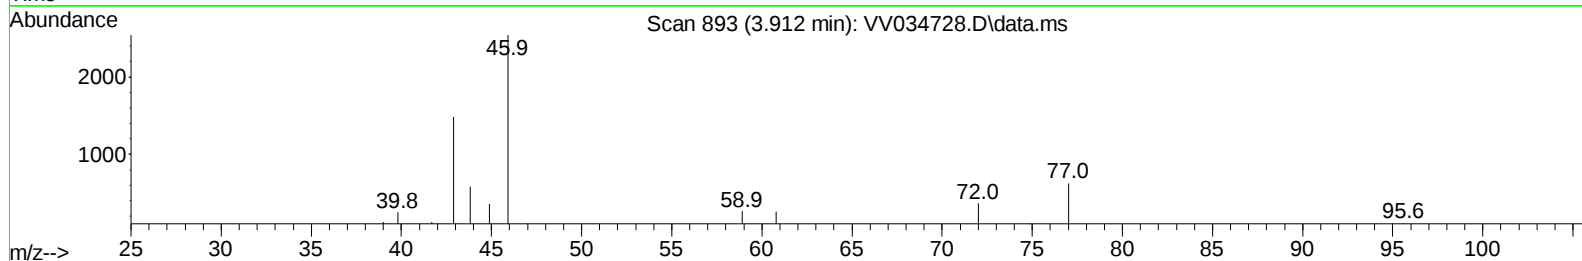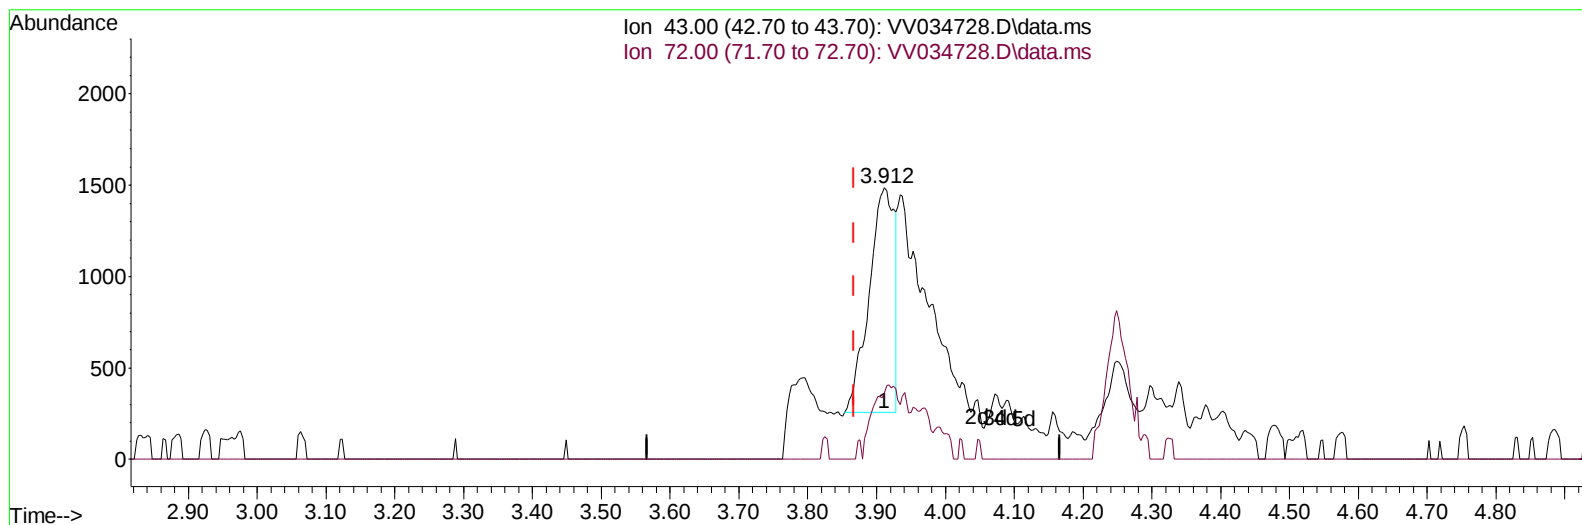

TIC: VV034728.D\data.ms

(22) 2-Butanone (T)

3.912min (+ 0.045) 1.52 ug/L

response 3119

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	22.90	6.03#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034728.D
Acq On : 19 Mar 2024 12:24
Operator : SY/MD
Sample : P1751-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL18

Manual IntegrationsAPPROVED

Quant Time: Mar 20 01:22:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/20/2024
Supervised By :Semsettin Yesilyurt 03/20/2024

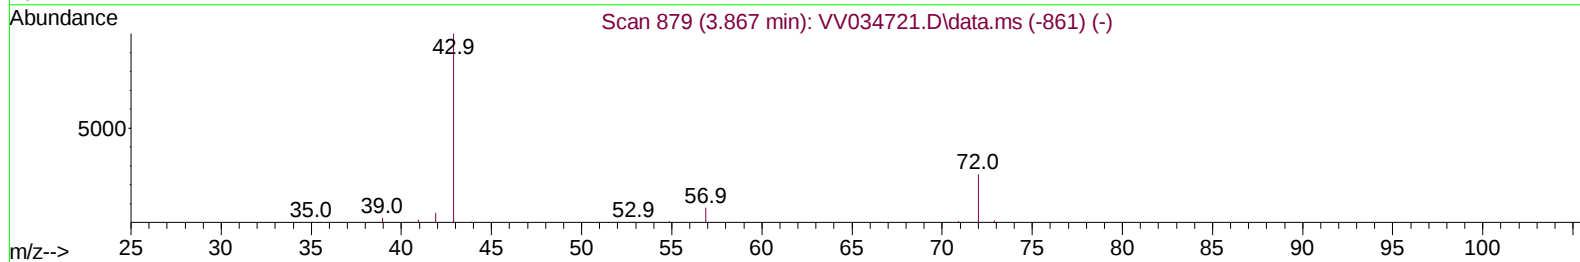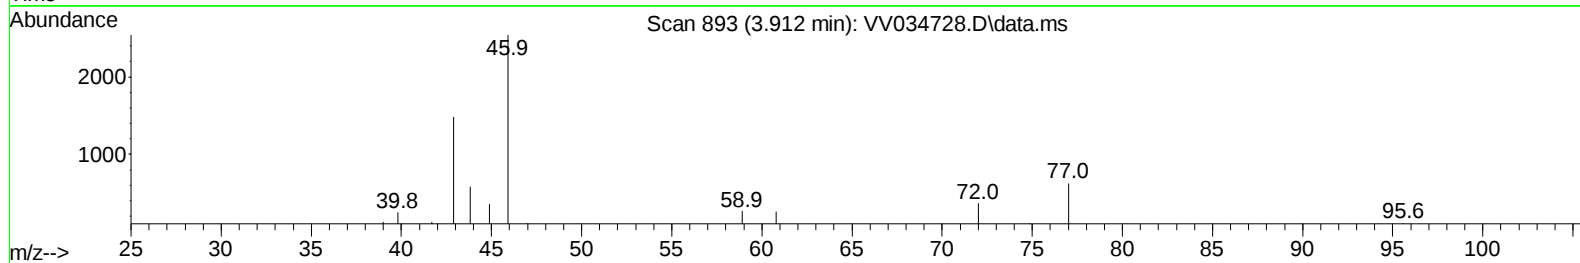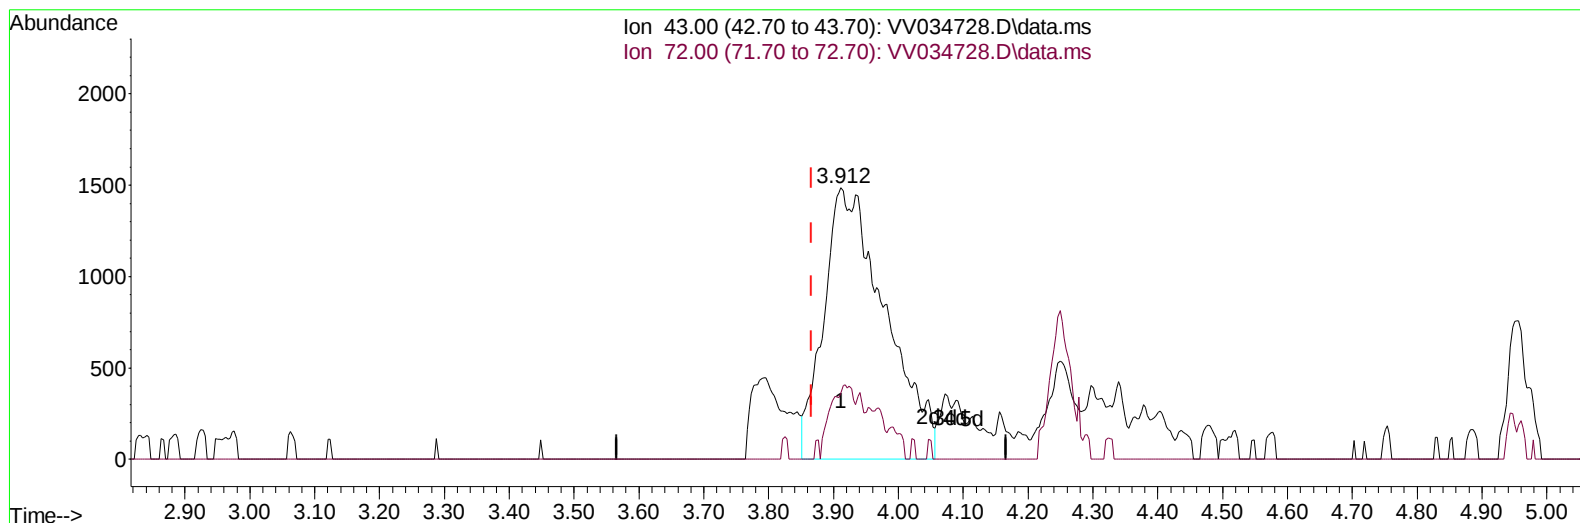

TIC: VV034728.D\data.ms

(22) 2-Butanone (T)

3.912min (+ 0.045) 4.78 ug/L m

response 9786

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	22.90	1.92#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034728.D
 Acq On : 19 Mar 2024 12:24
 Operator : SY/MD
 Sample : P1751-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL18

Manual IntegrationsAPPROVED

Quant Time: Mar 20 01:22:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/20/2024
 Supervised By :Semsettin Yesilyurt 03/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	297374	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	281549	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	131368	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	150880	58.528	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	117.060%	
7) Chloroethane-d5	1.532	69	122028	60.759	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	121.520%	
11) 1,1-Dichloroethene-d2	2.060	65	69229	59.380	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	118.760%	
21) 2-Butanone-d5	3.786	46	197168	114.369	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	114.370%	
24) Chloroform-d	4.246	84	260366	57.122	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	114.240%	
26) 1,2-Dichloroethane-d4	4.937	65	178922	60.070	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	120.140%	
32) Benzene-d6	4.957	84	517156	60.862	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	121.720%	
36) 1,2-Dichloropropane-d6	5.985	67	157235	60.634	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	121.260%#	
41) Toluene-d8	7.239	98	459766	59.791	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	119.580%	
43) trans-1,3-Dichloroprop...	7.551	79	75156	57.714	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	115.420%	
47) 2-Hexanone-d5	8.024	63	120502	93.057	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	93.060%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	204144	59.821	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	119.640%	
66) 1,2-Dichlorobenzene-d4	11.558	152	170473	63.486	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	126.980%#	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.069	96	79101	35.523	ug/L #	65
13) Acetone	2.117	43	277018	133.665	ug/L	99
19) 1,1-Dichloroethane	3.114	63	16298	3.860	ug/L	95
20) cis-1,2-Dichloroethene	3.815	96	22382	9.571	ug/L	92
22) 2-Butanone	3.912	43	9786m	4.782	ug/L	
30) 1,1,1-Trichloroethane	4.516	97	19476	4.824	ug/L	97
34) Trichloroethene	5.834	95	37453	15.077	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034728.D
Acq On : 19 Mar 2024 12:24
Operator : SY/MD
Sample : P1751-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL18

Manual IntegrationsAPPROVED

Quant Time: Mar 20 01:22:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/20/2024
Supervised By :Semsettin Yesilyurt 03/20/2024

