

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034733.D
 Acq On : 19 Mar 2024 14:23
 Operator : SY/MD
 Sample : P1751-20DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL45DL

Quant Time: Mar 20 01:23:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	333694	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	317095	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	146878	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	138761	47.968	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	95.940%	
7) Chloroethane-d5	1.532	69	112901	50.096	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	100.200%	
11) 1,1-Dichloroethene-d2	2.060	65	63056	48.199	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.400%	
21) 2-Butanone-d5	3.789	46	182168	94.167	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	94.170%	
24) Chloroform-d	4.246	84	247547	48.399	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	4.937	65	169128	50.601	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.200%	
32) Benzene-d6	4.957	84	492073	51.418	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.840%	
36) 1,2-Dichloropropane-d6	5.986	67	149186	51.081	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	102.160%	
41) Toluene-d8	7.243	98	434381	50.157	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.320%	
43) trans-1,3-Dichloroprop...	7.551	79	71799	48.955	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.920%	
47) 2-Hexanone-d5	8.024	63	112676	77.259	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	77.260%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	192615	50.115	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	100.240%	
66) 1,2-Dichlorobenzene-d4	11.558	152	157262	52.382	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.760%	
Target Compounds						
13) Acetone	2.121	43	119657	51.452	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034733.D
Acq On : 19 Mar 2024 14:23
Operator : SY/MD
Sample : P1751-20DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCL45DL

Quant Time: Mar 20 01:23:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

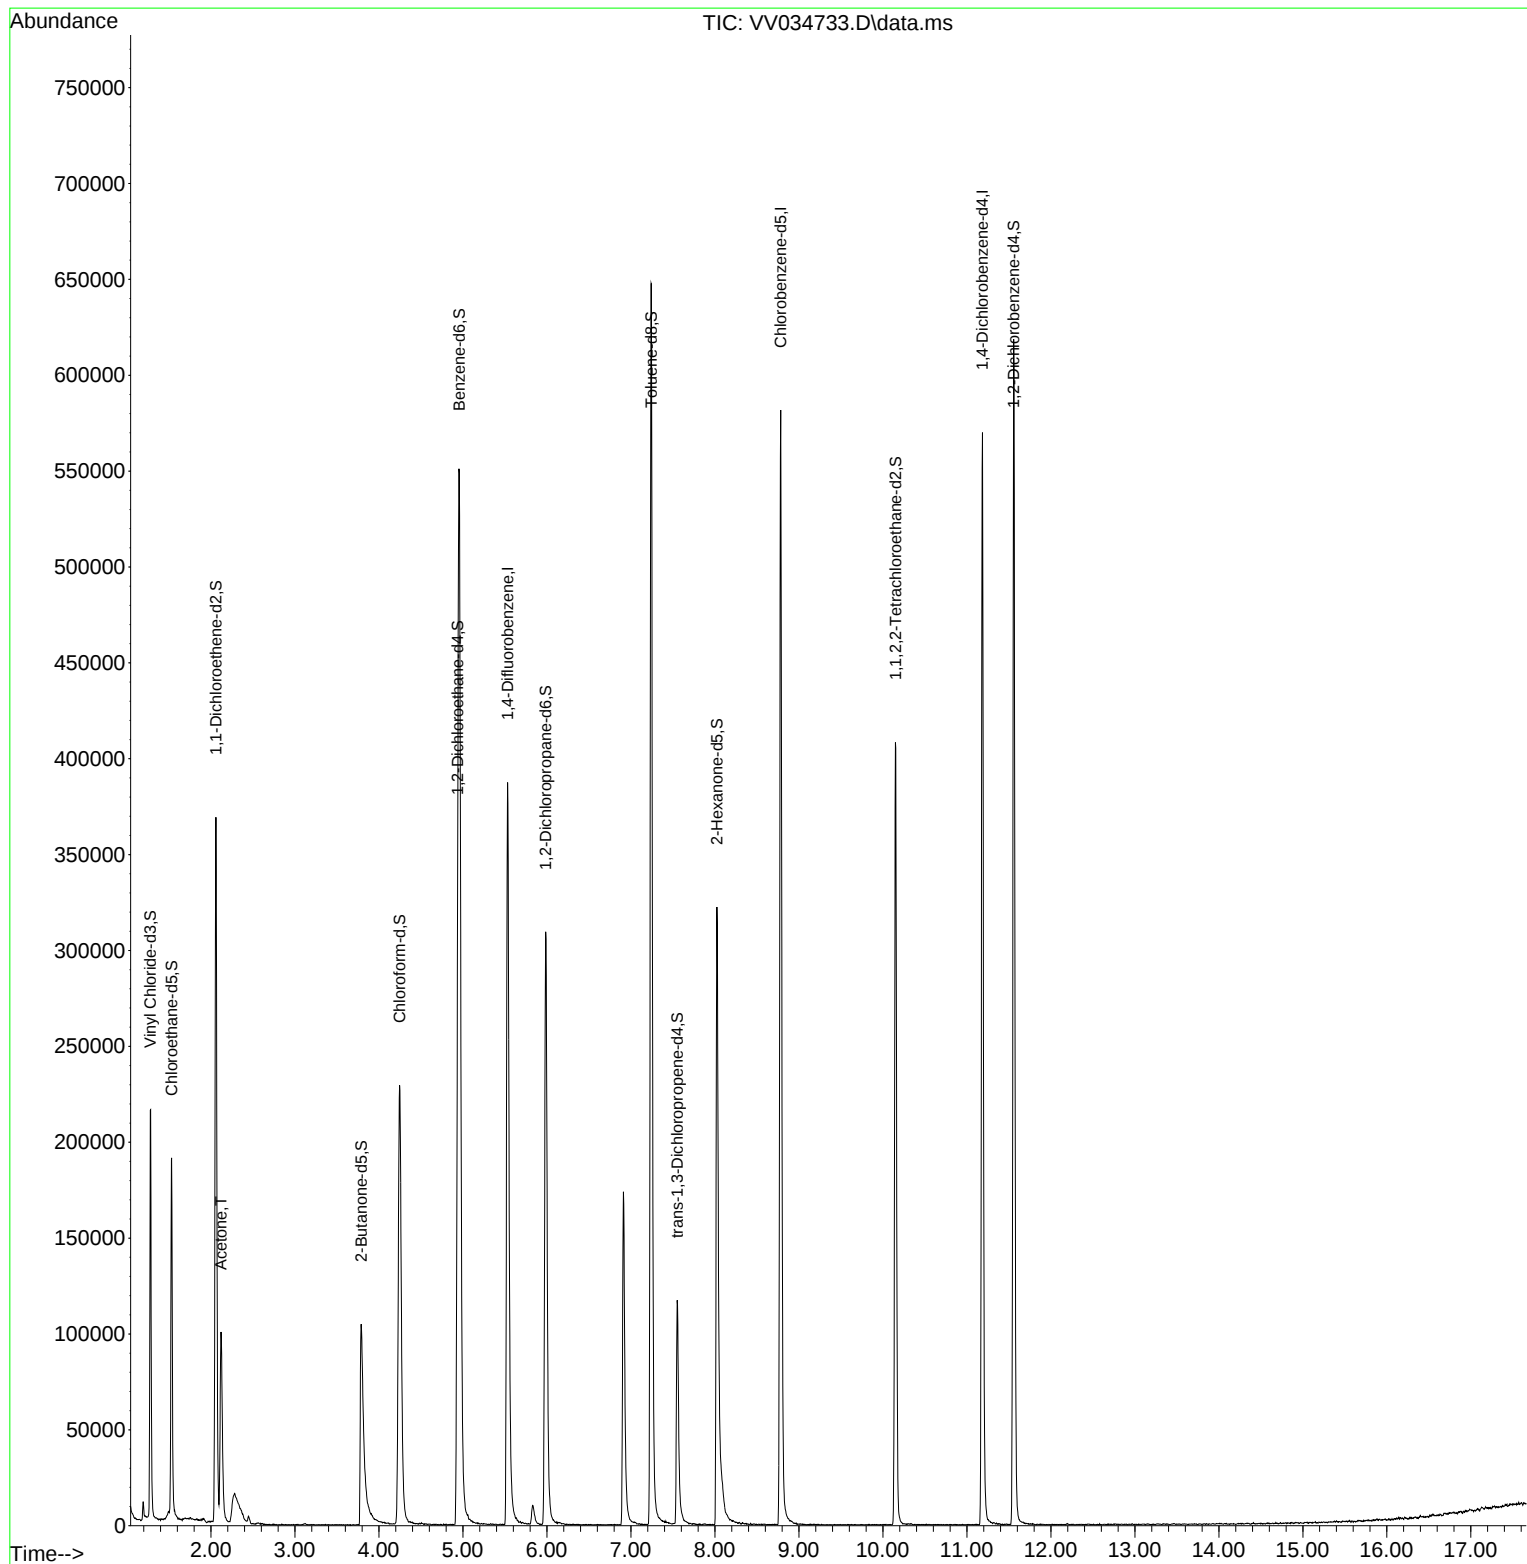

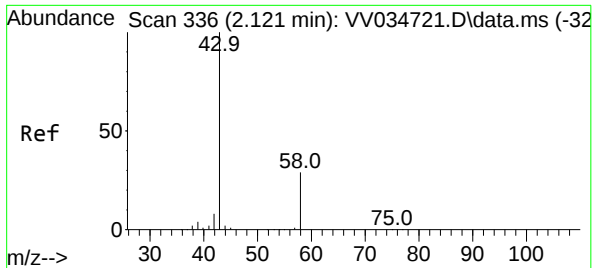

#13
 Acetone
 Concen: 51.452 ug/L
 RT: 2.121 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: VV034733.D
 Acq: 19 Mar 2024 14:23

Instrument :
 MSVOA_V
 ClientSampleId :
 YCL45DL

Tgt Ion: 43 Resp: 119657
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 57.2

