

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034742.D
 Acq On : 19 Mar 2024 17:57
 Operator : SY/MD
 Sample : P1755-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKT4

Quant Time: Mar 20 01:26:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	333460	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	316038	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	143309	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	128512	44.456	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	88.920%	
7) Chloroethane-d5	1.526	69	109332	48.547	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	97.100%	
11) 1,1-Dichloroethene-d2	2.056	65	57721	44.152	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.300%	
21) 2-Butanone-d5	3.786	46	176293	91.194	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	91.190%	
24) Chloroform-d	4.246	84	238708	46.703	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	4.937	65	161524	48.360	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.720%	
32) Benzene-d6	4.956	84	467002	48.962	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.920%	
36) 1,2-Dichloropropane-d6	5.985	67	146135	50.204	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	100.400%	
41) Toluene-d8	7.243	98	409837	47.481	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.960%	
43) trans-1,3-Dichloroprop...	7.551	79	69075	47.255	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	94.520%	
47) 2-Hexanone-d5	8.024	63	106386	73.191	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	73.190%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	186824	48.771	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	97.540%	
66) 1,2-Dichlorobenzene-d4	11.561	152	148783	50.792	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.580%	
Target Compounds						
13) Acetone	2.114	43	74776	32.176	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034742.D
Acq On : 19 Mar 2024 17:57
Operator : SY/MD
Sample : P1755-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKT4

Quant Time: Mar 20 01:26:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

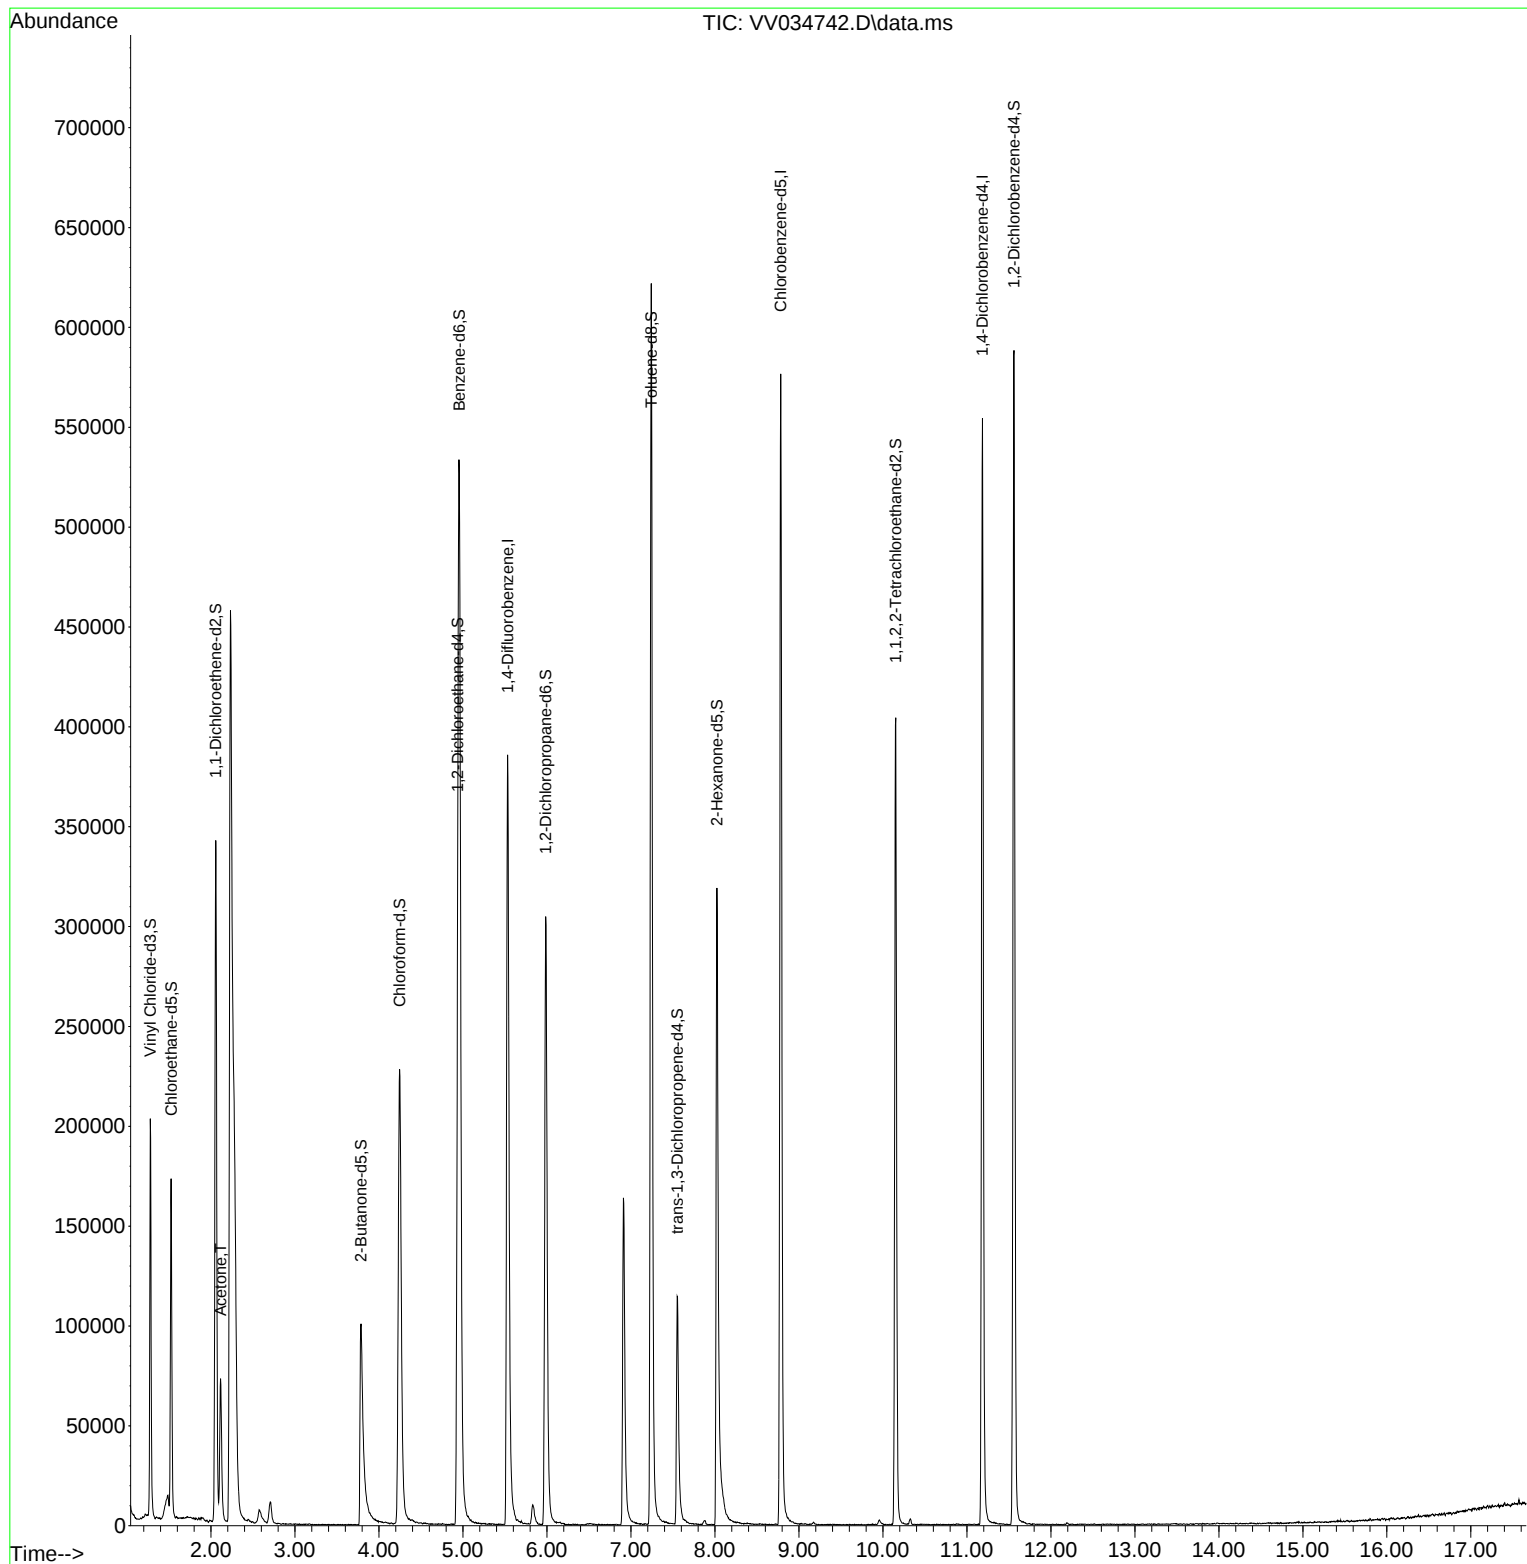

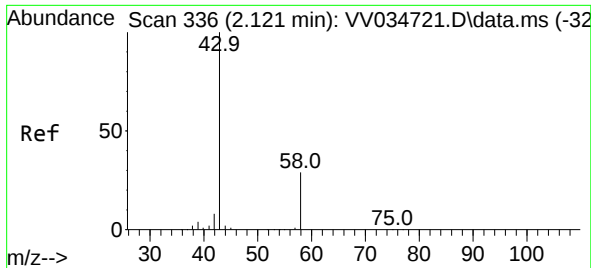

#13

Acetone

Concen: 32.176 ug/L

RT: 2.114 min Scan# 31

Delta R.T. -0.007 min

Lab File: VV034742.D

Acq: 19 Mar 2024 17:57

Instrument :

MSVOA_V

ClientSampleId :

YCKT4

Tgt Ion: 43 Resp: 74776

Ion Ratio Lower Upper

43 100

58 29.7 0.0 57.2

