

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031924\
 Data File : VW034743.D
 Acq On : 19 Mar 2024 18:21
 Operator : SY/MD
 Sample : P1755-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKT5

Quant Time: Mar 20 01:26:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	283117	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	272209	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	120825	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	106171	43.259	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.520%	
7) Chloroethane-d5	1.523	69	91432	47.818	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	95.640%	
11) 1,1-Dichloroethene-d2	2.057	65	47500	42.794	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	85.580%	
21) 2-Butanone-d5	3.786	46	171584	104.541	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	104.540%	
24) Chloroform-d	4.246	84	211925	48.836	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.680%	
26) 1,2-Dichloroethane-d4	4.941	65	146403	51.627	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.260%	
32) Benzene-d6	4.957	84	408437	49.716	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.440%	
36) 1,2-Dichloropropane-d6	5.986	67	129746	51.750	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	103.500%	
41) Toluene-d8	7.243	98	356363	47.934	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.860%	
43) trans-1,3-Dichloroprop...	7.551	79	61281	48.674	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.340%	
47) 2-Hexanone-d5	8.024	63	102234	81.659	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	81.660%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84	173491	52.583	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	105.160%	
66) 1,2-Dichlorobenzene-d4	11.561	152	130996	53.041	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	106.080%	
Target Compounds						
13) Acetone	2.114	43	56022	28.393	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034743.D
Acq On : 19 Mar 2024 18:21
Operator : SY/MD
Sample : P1755-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCKT5

Quant Time: Mar 20 01:26:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

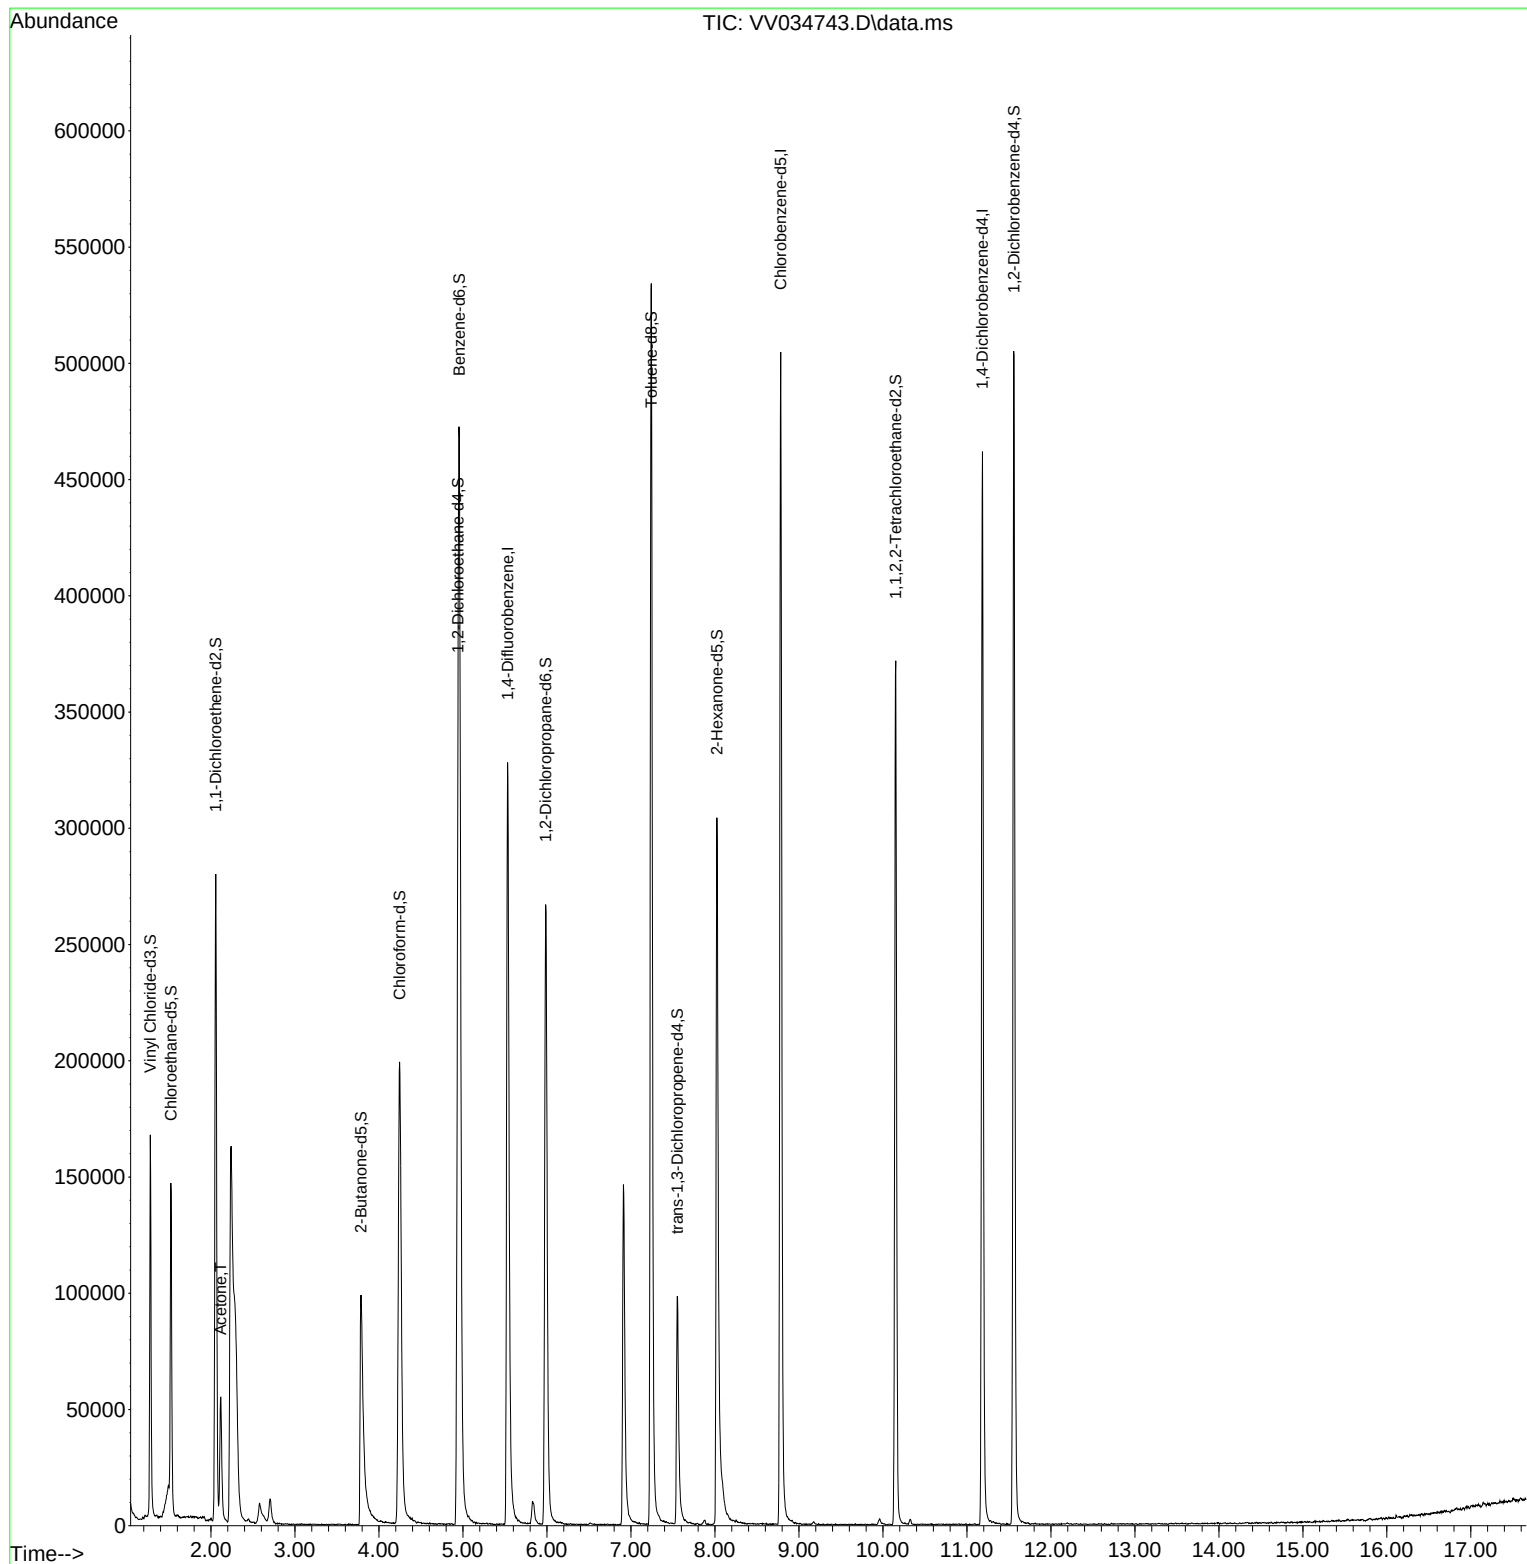

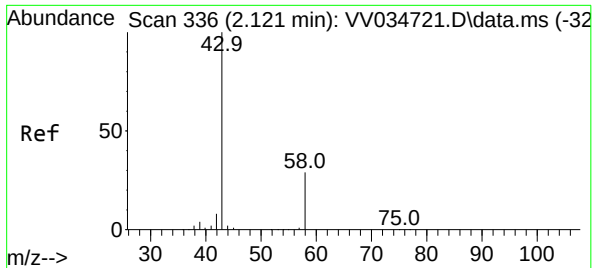

#13
 Acetone
 Concen: 28.393 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV034743.D
 Acq: 19 Mar 2024 18:21

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKT5

Tgt Ion: 43 Resp: 56022
 Ion Ratio Lower Upper
 43 100
 58 29.9 0.0 57.2

