

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034744.D
 Acq On : 19 Mar 2024 18:45
 Operator : SY/MD
 Sample : P1755-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKW0

Quant Time: Mar 20 01:26:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 20 01:19:21 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 03/20/2024
 Supervised By :Semsettin Yesilyurt 03/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	336144	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	316927	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	145682	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	131468	45.116	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.240%		
7) Chloroethane-d5	1.529	69	110131m	48.511	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	97.020%		
11) 1,1-Dichloroethene-d2	2.060	65	59840	45.407	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.820%		
21) 2-Butanone-d5	3.786	46	176497	90.571	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.570%		
24) Chloroform-d	4.246	84	238774	46.343	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.680%		
26) 1,2-Dichloroethane-d4	4.941	65	161913	48.090	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.180%		
32) Benzene-d6	4.960	84	466519	48.774	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.540%		
36) 1,2-Dichloropropane-d6	5.985	67	146367	50.142	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.280%		
41) Toluene-d8	7.243	98	412566	47.663	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.320%		
43) trans-1,3-Dichloroprop...	7.551	79	68573	46.780	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.560%		
47) 2-Hexanone-d5	8.024	63	106719	73.214	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	73.210%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	188924	49.181	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.360%		
66) 1,2-Dichlorobenzene-d4	11.561	152	154756	51.970	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.940%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	228629	97.593	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034744.D
Acq On : 19 Mar 2024 18:45
Operator : SY/MD
Sample : P1755-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
YCKW0

Quant Time: Mar 20 01:26:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 20 01:19:21 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 03/20/2024
Supervised By :Semsettin Yesilyurt 03/20/2024

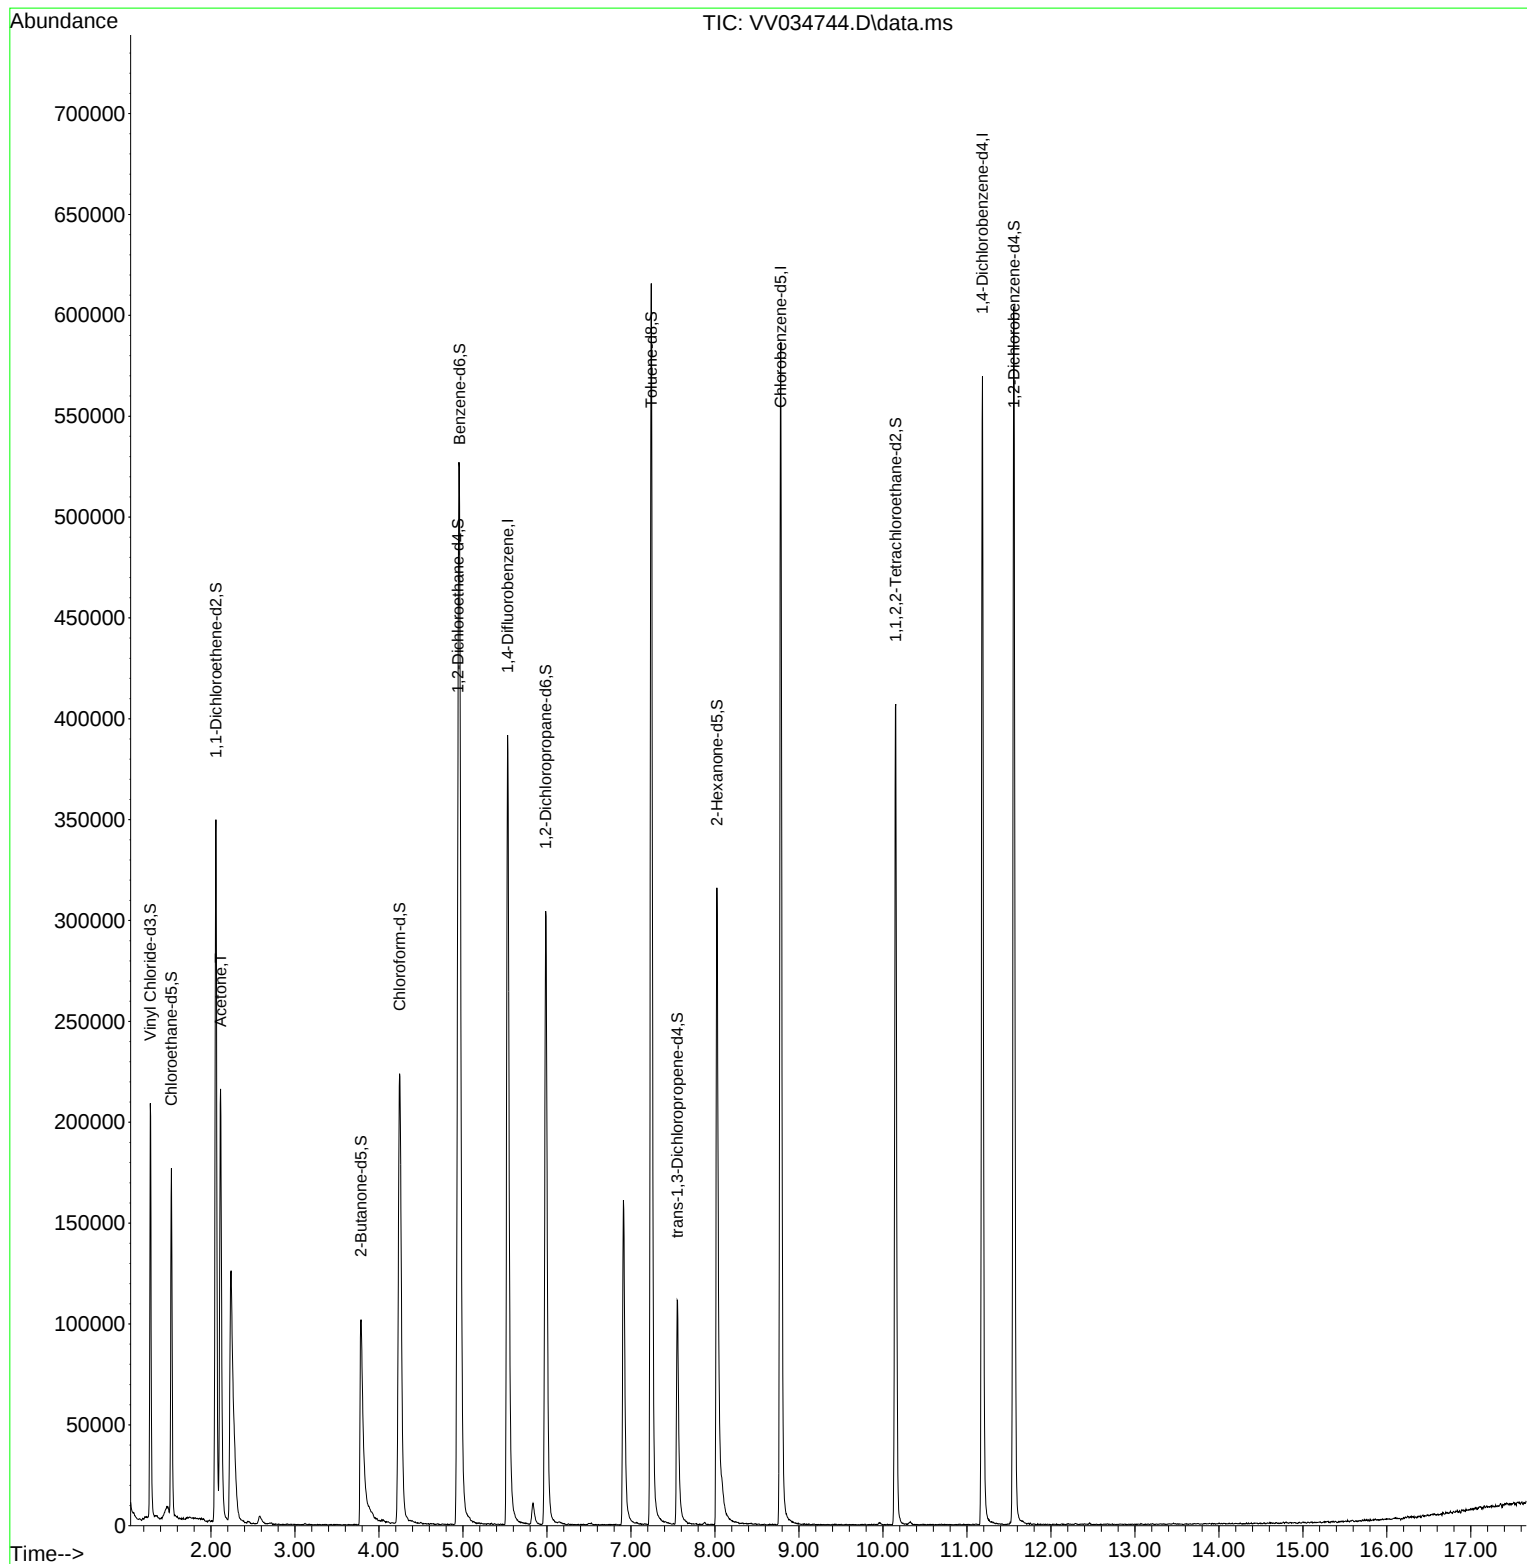

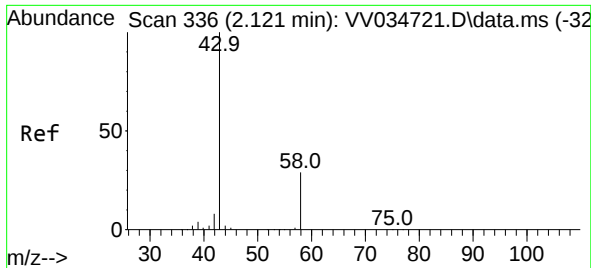

#13
 Acetone
 Concen: 97.593 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV034744.D
 Acq: 19 Mar 2024 18:45

Instrument :
 MSVOA_V
 ClientSampleId :
 YCKW0

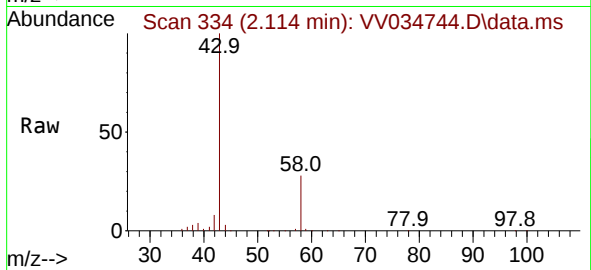

Tgt Ion: 43 Resp: 228629
 Ion Ratio Lower Upper
 43 100
 58 28.6 0.0 57.2

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 03/20/2024
 Supervised By :Semsettin Yesilyurt 03/20/2024

