

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034696.D
 Acq On : 18 Mar 2024 15:07
 Operator : SY/MD
 Sample : VV0319WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rVB	259631	274596	16.64%	2.284%
2	1.532	146	153	167	rVB	207239	240612	14.58%	2.001%
3	2.060	307	317	335	rBV	417869	605460	36.69%	5.036%
4	2.375	412	415	417	rBV	305	241	0.01%	0.002%
5	2.452	430	439	447	rBV6	2250	3689	0.22%	0.031%
6	2.661	501	504	506	rBV2	330	206	0.01%	0.002%
7	2.725	521	524	526	rBV	219	136	0.01%	0.001%
8	2.777	535	540	542	rBV2	344	331	0.02%	0.003%
9	2.957	593	596	597	rBV	255	140	0.01%	0.001%
10	3.005	608	611	613	rBV	216	163	0.01%	0.001%
11	3.063	626	629	635	rBV2	231	265	0.02%	0.002%
12	3.092	635	638	640	rVV2	183	116	0.01%	0.001%
13	3.105	640	642	645	rVB	231	104	0.01%	0.001%
14	3.198	668	671	674	rBV2	127	119	0.01%	0.001%
15	3.240	681	684	686	rBV	143	99	0.01%	0.001%
16	3.336	709	714	715	rBV	178	151	0.01%	0.001%
17	3.449	747	749	751	rBV	151	80	0.00%	0.001%
18	3.490	760	762	766	rVB2	373	243	0.01%	0.002%
19	3.516	766	770	774	rBV2	182	187	0.01%	0.002%
20	3.545	776	779	783	rBV2	112	99	0.01%	0.001%
21	3.793	847	856	903	rBV	114412	338057	20.48%	2.812%
22	4.249	983	998	1027	rBV	252485	647316	39.22%	5.384%
23	4.786	1161	1165	1172	rVB2	327	328	0.02%	0.003%
24	4.821	1173	1176	1180	rBV2	294	220	0.01%	0.002%
25	4.870	1189	1191	1194	rBV2	311	216	0.01%	0.002%
26	4.957	1201	1218	1259	rBV2	627140	1650285	100.00%	13.726%
27	5.330	1329	1334	1337	rBV	475	488	0.03%	0.004%
28	5.403	1350	1357	1359	rBV2	383	418	0.03%	0.003%
29	5.420	1359	1362	1365	rVB	575	339	0.02%	0.003%
30	5.445	1368	1370	1373	rBV	246	128	0.01%	0.001%
31	5.468	1375	1377	1378	rBV	202	72	0.00%	0.001%
32	5.532	1385	1397	1434	rBV	426734	889269	53.89%	7.397%
33	5.831	1480	1490	1512	rBV4	12434	27564	1.67%	0.229%
34	5.989	1525	1539	1571	rBV	350949	729320	44.19%	6.066%
35	6.291	1629	1633	1634	rBV2	211	141	0.01%	0.001%
36	6.317	1639	1641	1642	rBV	282	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034696.D
 Acq On : 18 Mar 2024 15:07
 Operator : SY/MD
 Sample : VV0319WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.458	1683	1685	1687	rBV	140	80	0.00%	0.001%
38	6.580	1718	1723	1725	rBV	252	242	0.01%	0.002%
39	6.616	1728	1734	1736	rVV	359	258	0.02%	0.002%
40	6.667	1747	1750	1753	rBV2	303	161	0.01%	0.001%
41	6.683	1753	1755	1759	rVV2	108	76	0.00%	0.001%
42	6.786	1785	1787	1792	rBV2	199	143	0.01%	0.001%
43	6.847	1800	1806	1808	rBV4	324	317	0.02%	0.003%
44	6.863	1808	1811	1815	rVB2	217	146	0.01%	0.001%
45	6.911	1815	1826	1853	rBV	195334	371925	22.54%	3.093%
46	7.146	1896	1899	1901	rBV2	416	318	0.02%	0.003%
47	7.198	1910	1915	1917	rBV3	522	531	0.03%	0.004%
48	7.243	1918	1929	1967	rVV	744446	1310770	79.43%	10.902%
49	7.551	2016	2025	2061	rBV	131505	244725	14.83%	2.036%
50	7.744	2083	2085	2087	rBV2	571	296	0.02%	0.002%
51	7.860	2118	2121	2123	rBV	331	216	0.01%	0.002%
52	7.911	2135	2137	2141	rBV	174	127	0.01%	0.001%
53	7.960	2149	2152	2155	rVB2	259	163	0.01%	0.001%
54	7.972	2155	2156	2159	rVB	146	74	0.00%	0.001%
55	8.024	2163	2172	2213	rBV	370012	717370	43.47%	5.967%
56	8.519	2321	2326	2329	rBV3	402	434	0.03%	0.004%
57	8.622	2356	2358	2360	rBV2	228	84	0.01%	0.001%
58	8.677	2373	2375	2381	rVB	283	254	0.02%	0.002%
59	8.718	2386	2388	2390	rBV2	183	113	0.01%	0.001%
60	8.783	2396	2408	2432	rBV	634834	1041684	63.12%	8.664%
61	9.098	2501	2506	2507	rBV2	270	228	0.01%	0.002%
62	9.165	2524	2527	2530	rBV2	240	143	0.01%	0.001%
63	9.223	2541	2545	2549	rBV4	378	341	0.02%	0.003%
64	9.243	2549	2551	2555	rVB	250	125	0.01%	0.001%
65	9.304	2568	2570	2572	rBV	236	109	0.01%	0.001%
66	9.500	2629	2631	2634	rBV	182	72	0.00%	0.001%
67	9.519	2635	2637	2640	rBV	189	135	0.01%	0.001%
68	9.593	2658	2660	2663	rBV	208	96	0.01%	0.001%
69	9.686	2685	2689	2694	rBV2	177	214	0.01%	0.002%
70	9.882	2747	2750	2756	rBV2	299	300	0.02%	0.002%
71	10.152	2822	2834	2858	rBV	447574	709137	42.97%	5.898%
72	10.323	2885	2887	2894	rVB2	780	595	0.04%	0.005%
73	10.390	2904	2908	2910	rBV	196	158	0.01%	0.001%
74	10.487	2932	2938	2941	rBV2	384	466	0.03%	0.004%
75	10.532	2949	2952	2954	rBV	234	160	0.01%	0.001%
76	10.741	3014	3017	3021	rBV2	197	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
 Data File : VV034696.D
 Acq On : 18 Mar 2024 15:07
 Operator : SY/MD
 Sample : VV0319WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.789	3031	3032	3036	rVB	231	87	0.01%	0.001%
78	10.828	3040	3044	3047	rBV	307	259	0.02%	0.002%
79	10.866	3052	3056	3065	rBV2	521	561	0.03%	0.005%
80	10.979	3089	3091	3093	rBV2	201	101	0.01%	0.001%
81	11.107	3128	3131	3134	rVB	471	285	0.02%	0.002%
82	11.127	3135	3137	3138	rBV	227	92	0.01%	0.001%
83	11.185	3143	3155	3188	rVV	656610	1034081	62.66%	8.601%
84	11.423	3227	3229	3230	rBV	346	123	0.01%	0.001%
85	11.503	3251	3254	3255	rBV	231	104	0.01%	0.001%
86	11.558	3259	3271	3292	rBV	730847	1159591	70.27%	9.645%
87	11.873	3367	3369	3371	rVV	343	135	0.01%	0.001%
88	11.950	3389	3393	3398	rBV2	320	368	0.02%	0.003%
89	12.091	3431	3437	3442	rVB2	345	346	0.02%	0.003%
90	12.120	3442	3446	3448	rBV2	408	318	0.02%	0.003%
91	12.191	3464	3468	3475	rBV2	527	611	0.04%	0.005%
92	12.426	3539	3541	3547	rVB2	423	271	0.02%	0.002%
93	12.738	3636	3638	3643	rVB	211	163	0.01%	0.001%
94	12.911	3690	3692	3694	rBV	217	108	0.01%	0.001%
95	13.136	3759	3762	3767	rBV	437	394	0.02%	0.003%
96	13.207	3780	3784	3785	rBV	1076	701	0.04%	0.006%
97	13.348	3821	3828	3831	rBV2	537	621	0.04%	0.005%
98	13.455	3853	3861	3870	rBV2	4249	6304	0.38%	0.052%
99	13.554	3890	3892	3895	rBV	288	111	0.01%	0.001%
100	13.686	3927	3933	3949	rVB7	1359	2843	0.17%	0.024%




Sum of corrected areas: 12022835

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034696.D
Acq On : 18 Mar 2024 15:07
Operator : SY/MD
Sample : VV0319WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

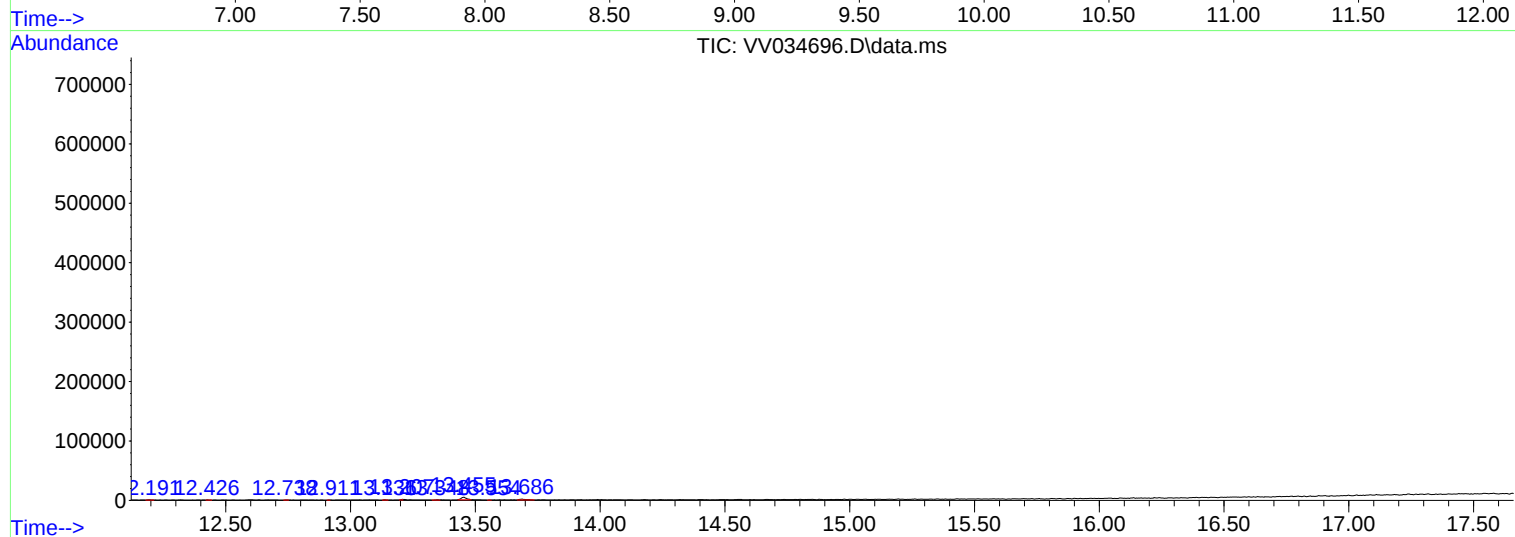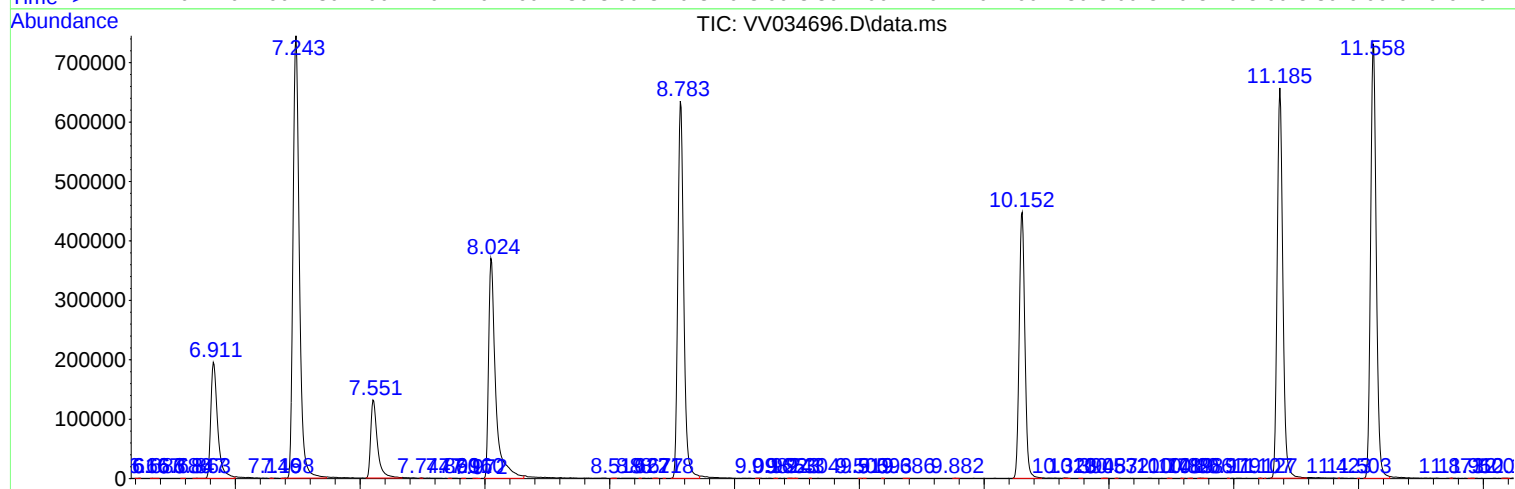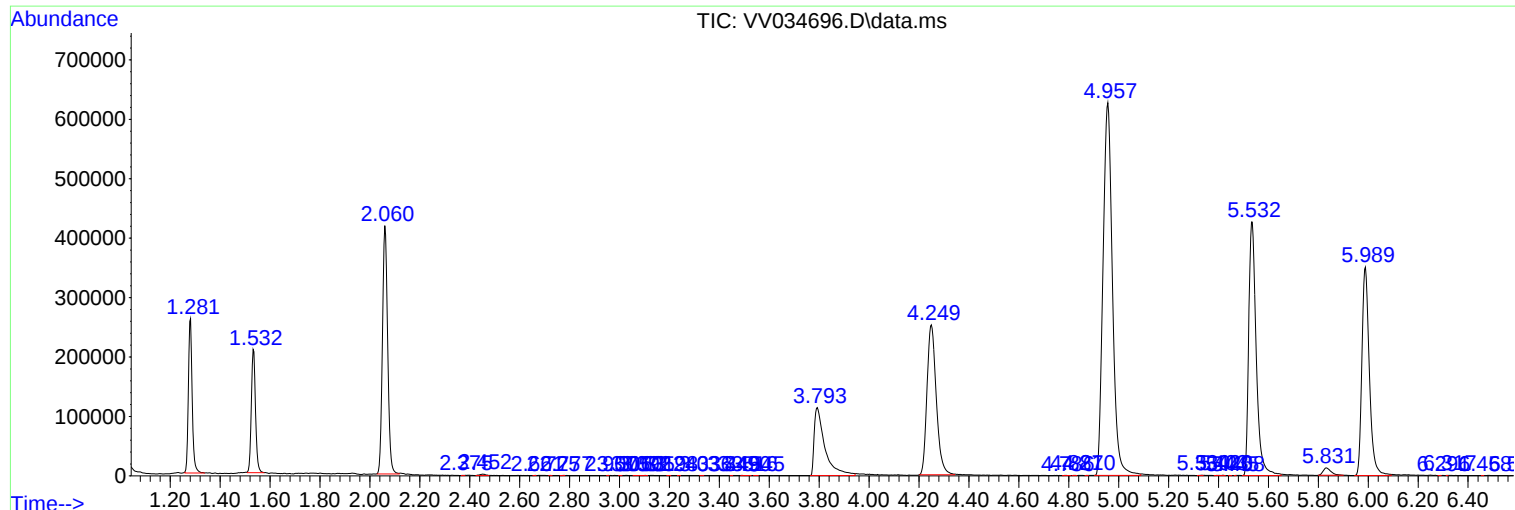

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034696.D
Acq On : 18 Mar 2024 15:07
Operator : SY/MD
Sample : VV0319WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031924\
Data File : VV034696.D
Acq On : 18 Mar 2024 15:07
Operator : SY/MD
Sample : VV0319WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc